

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100615\
Data File : HN007575.D
Signal(s) : vwd1A.ch
Acq On : 06-Oct-2015, 11:50
Operator : UM/MA
Sample : SSTDICC001
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
SSTDICC001

Integration File: AUTOINT1.E
Quant Time: Oct 06 17:22:16 2015
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN1006NG.M
Quant Title :
QLast Update : Tue Oct 06 17:22:00 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.330	4900038	1.255 ng/ul
Target Compounds			
2) T Nitroglycerin	6.018	10574376	1.313 ng/ul

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100615\
Data File : HN007575.D
Signal(s) : vwd1A.ch
Acq On : 06-Oct-2015, 11:50
Operator : UM/MA
Sample : SSTDICC001
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
SSTDICC001

Integration File: AUTOINT1.E
Quant Time: Oct 06 17:22:16 2015
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN1006NG.M
Quant Title :
QLast Update : Tue Oct 06 17:22:00 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

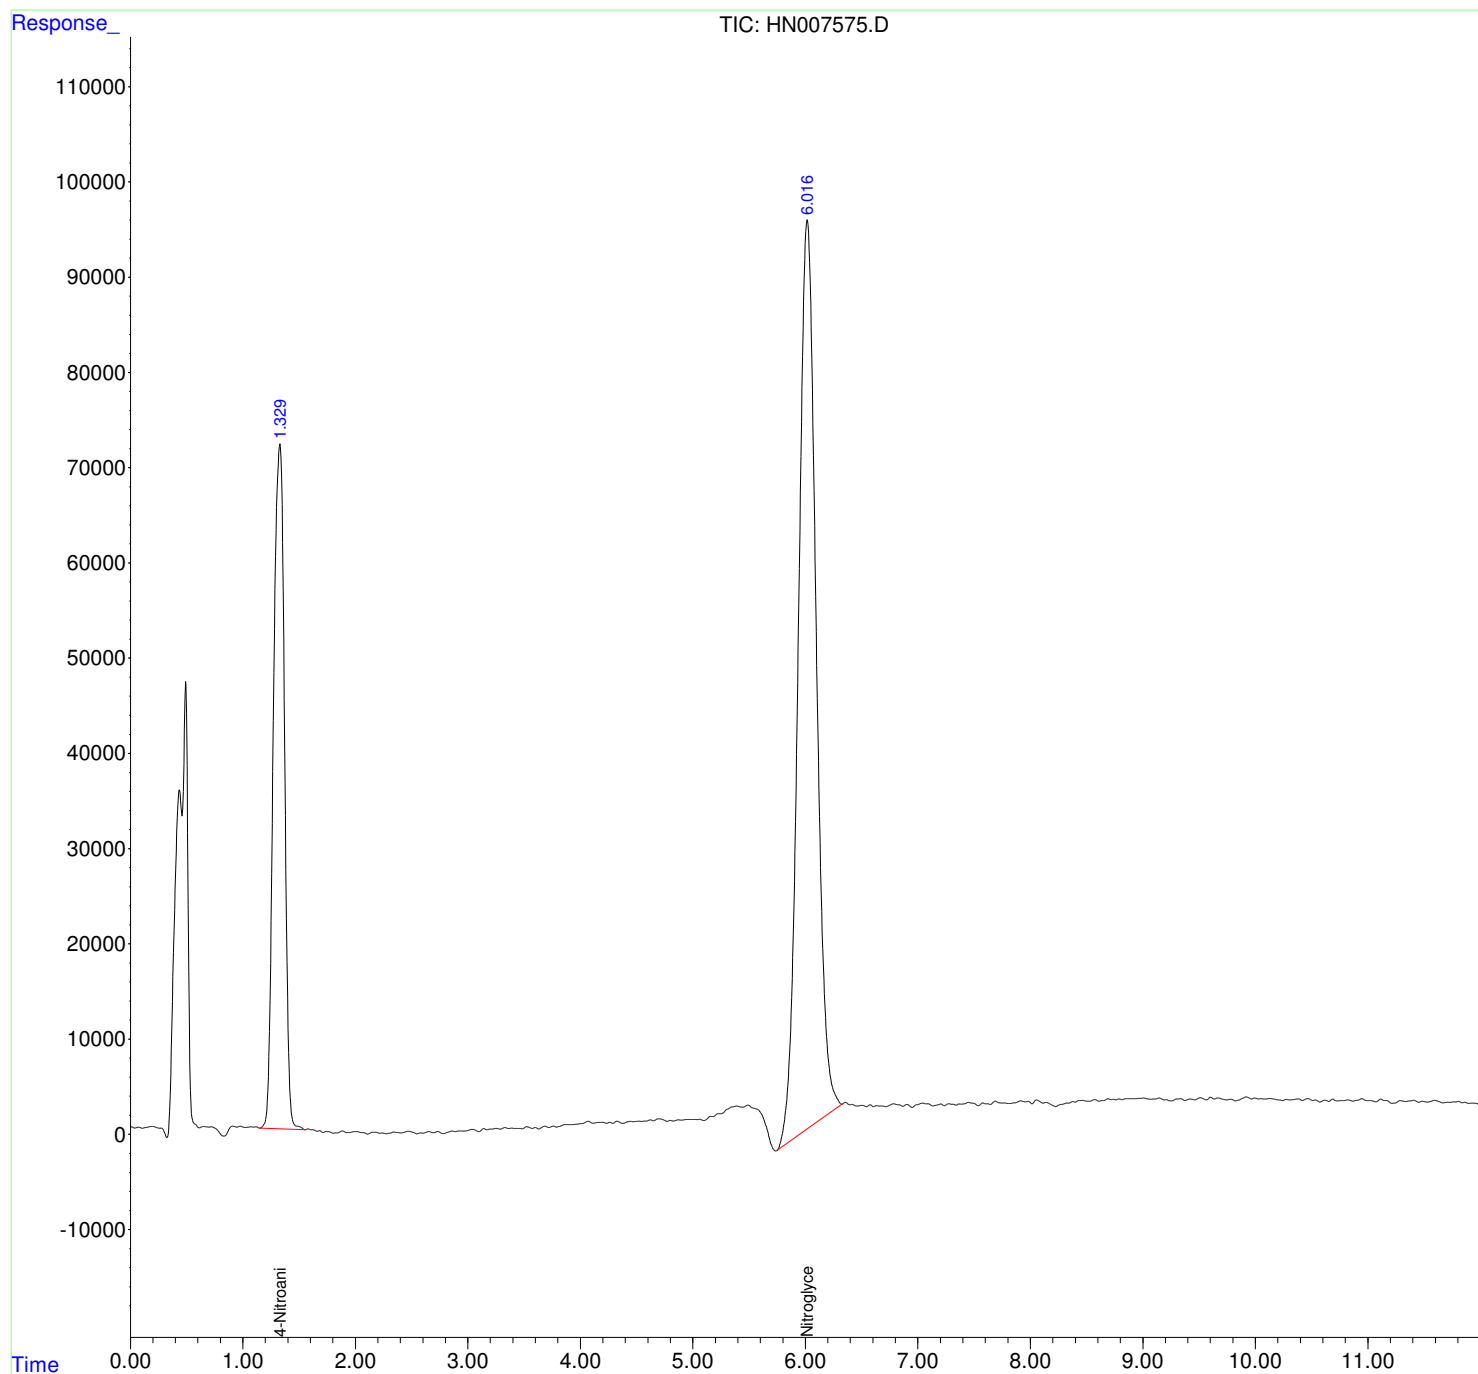


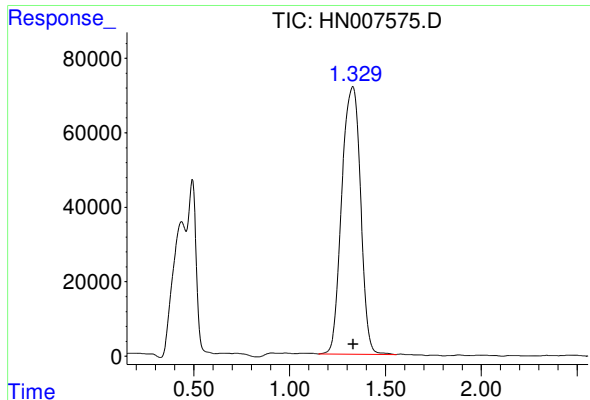

#1 4-Nitroaniline

R.T.: 1.330 min
Delta R.T.: 0.000 min
Response: 4900038
Conc: 1.25 ng/u1

Instrument :
HPLC_N
ClientSampleId :
SSTDICC001

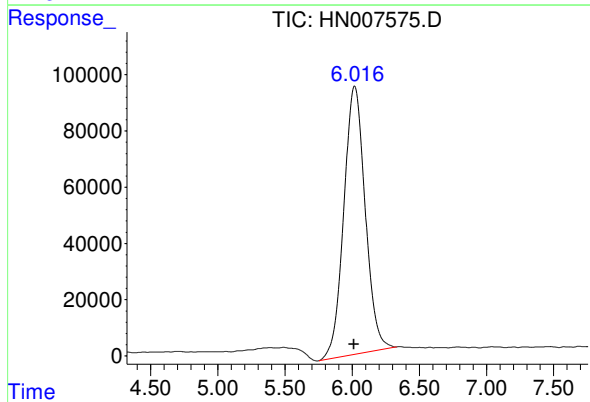

#2 Nitroglycerin

R.T.: 6.018 min
Delta R.T.: 0.007 min
Response: 10574376
Conc: 1.31 ng/u1