

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100615\
Data File : HN007576.D
Signal(s) : vwd1A.ch
Acq On : 06-Oct-2015, 16:10
Operator : UM/MA
Sample : SSTDICC0.5
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
SSTDICC0.5

Integration File: AUTOINT1.E
Quant Time: Oct 06 17:23:38 2015
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN1006NG.M
Quant Title :
QLast Update : Tue Oct 06 17:23:18 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.322	1745391	0.436 ng/ul
Target Compounds			
2) T Nitroglycerin	6.014	3995303	0.472 ng/ul

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100615\
Data File : HN007576.D
Signal(s) : vwd1A.ch
Acq On : 06-Oct-2015, 16:10
Operator : UM/MA
Sample : SSTDICC0.5
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
SSTDICC0.5

Integration File: AUTOINT1.E
Quant Time: Oct 06 17:23:38 2015
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN1006NG.M
Quant Title :
QLast Update : Tue Oct 06 17:23:18 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

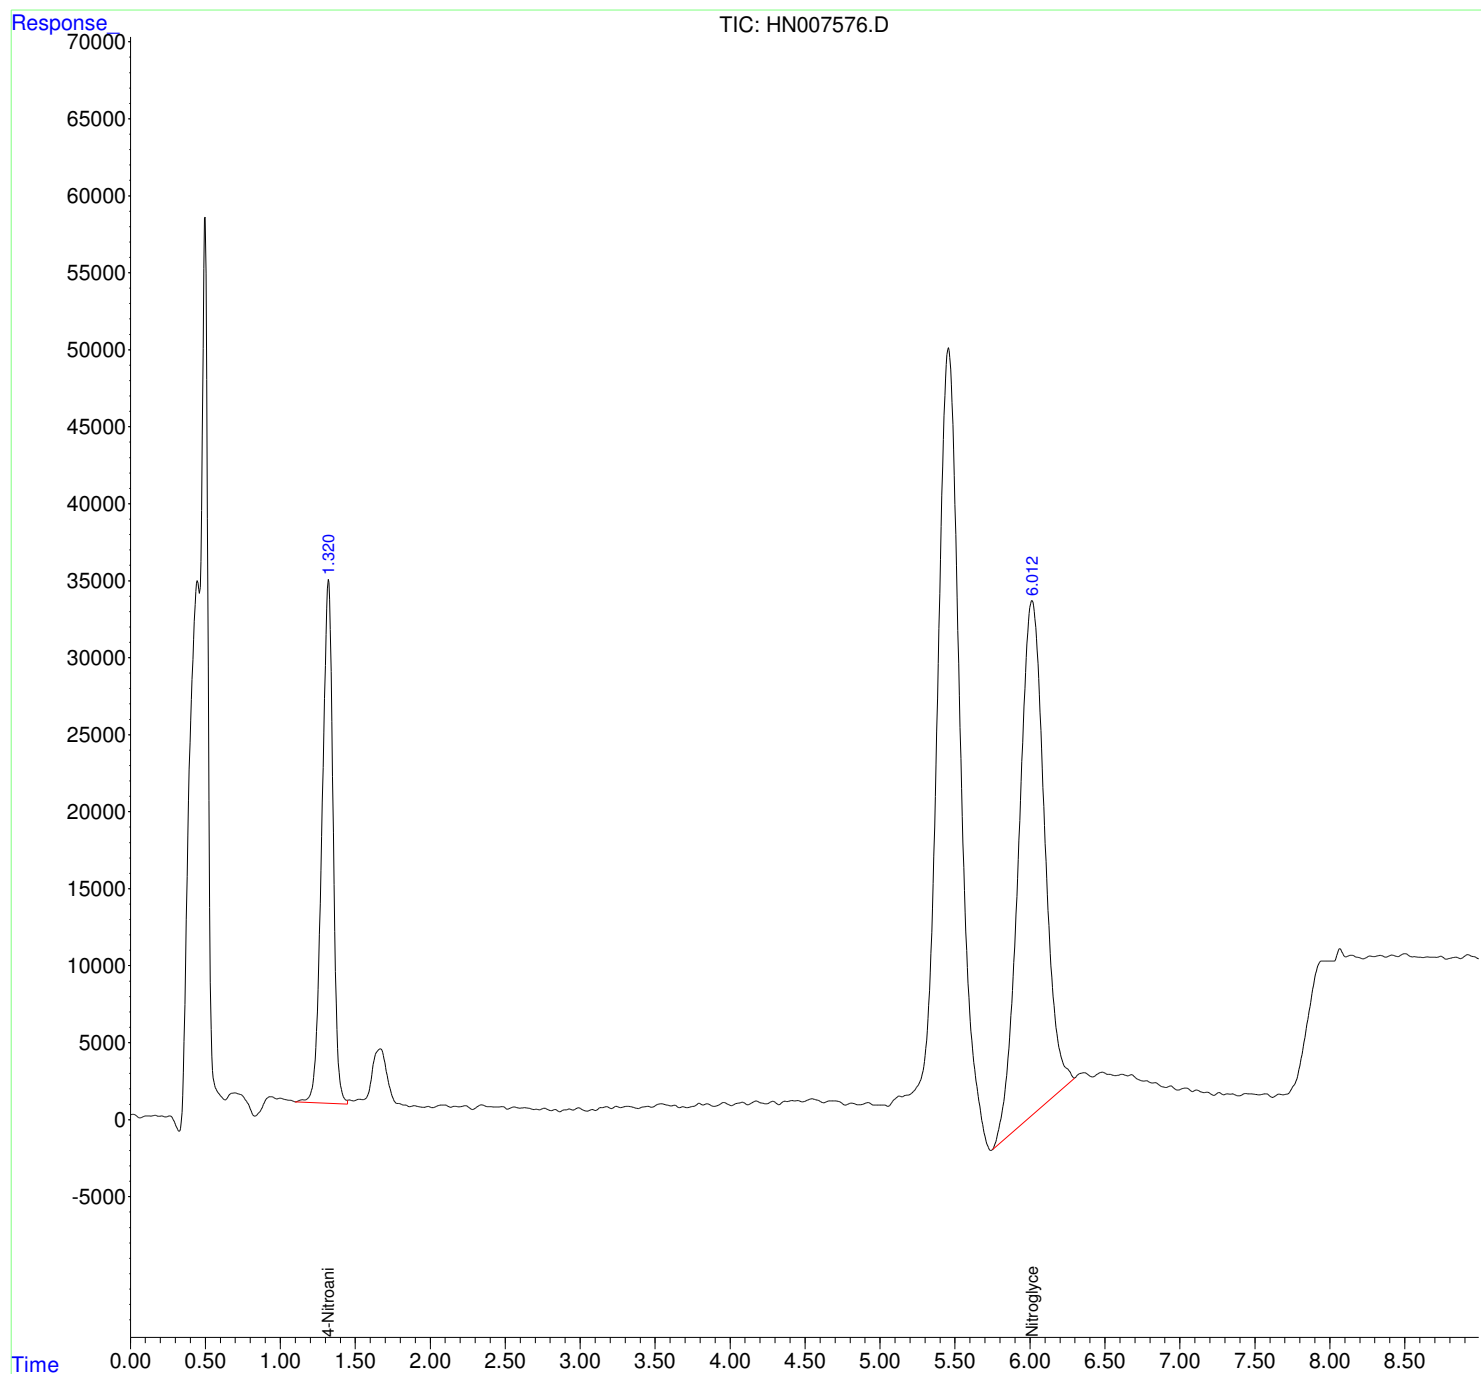


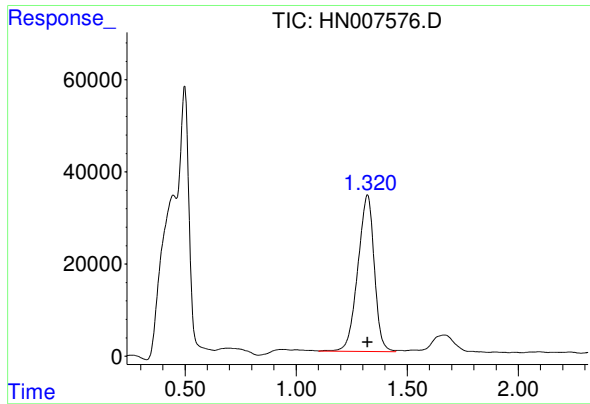

#1 4-Nitroaniline

R.T.: 1.322 min
Delta R.T.: 0.000 min
Response: 1745391
Conc: 0.44 ng/u1

Instrument :
HPLC_N
ClientSampleId :
SSTDICC0.5

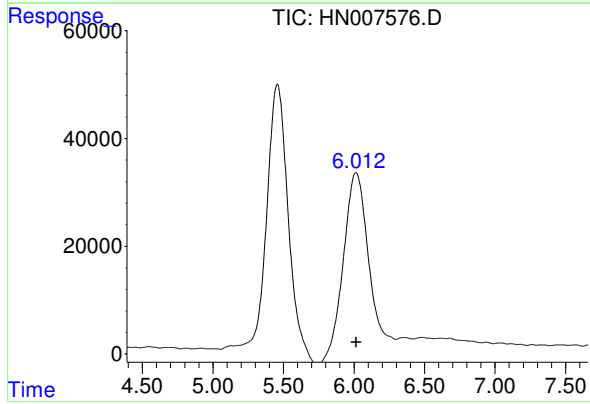

#2 Nitroglycerin

R.T.: 6.014 min
Delta R.T.: 0.000 min
Response: 3995303
Conc: 0.47 ng/u1