

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100615\
Data File : HN007577.D
Signal(s) : vwd1A.ch
Acq On : 06-Oct-2015, 17:44
Operator : UM/MA
Sample : SSTDICV005
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
SSTDICV005

Integration File: AUTOINT1.E
Quant Time: Oct 06 18:09:56 2015
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN1006NG.M
Quant Title :
QLast Update : Tue Oct 06 17:23:55 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.331	19440390	4.857 ng/ul
Target Compounds			
2) T Nitroglycerin	6.016	40534660	4.790 ng/ul

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN100615\
Data File : HN007577.D
Signal(s) : vwd1A.ch
Acq On : 06-Oct-2015, 17:44
Operator : UM/MA
Sample : SSTDICV005
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
SSTDICV005

Integration File: AUTOINT1.E
Quant Time: Oct 06 18:09:56 2015
Quant Method : Z:\HPCHEM1\HPLC_N\Methods\HN1006NG.M
Quant Title :
QLast Update : Tue Oct 06 17:23:55 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal Phase : ZORBAX Extend-C18
Signal Info : 4.6 X 100mm 3.5-Micron 80A

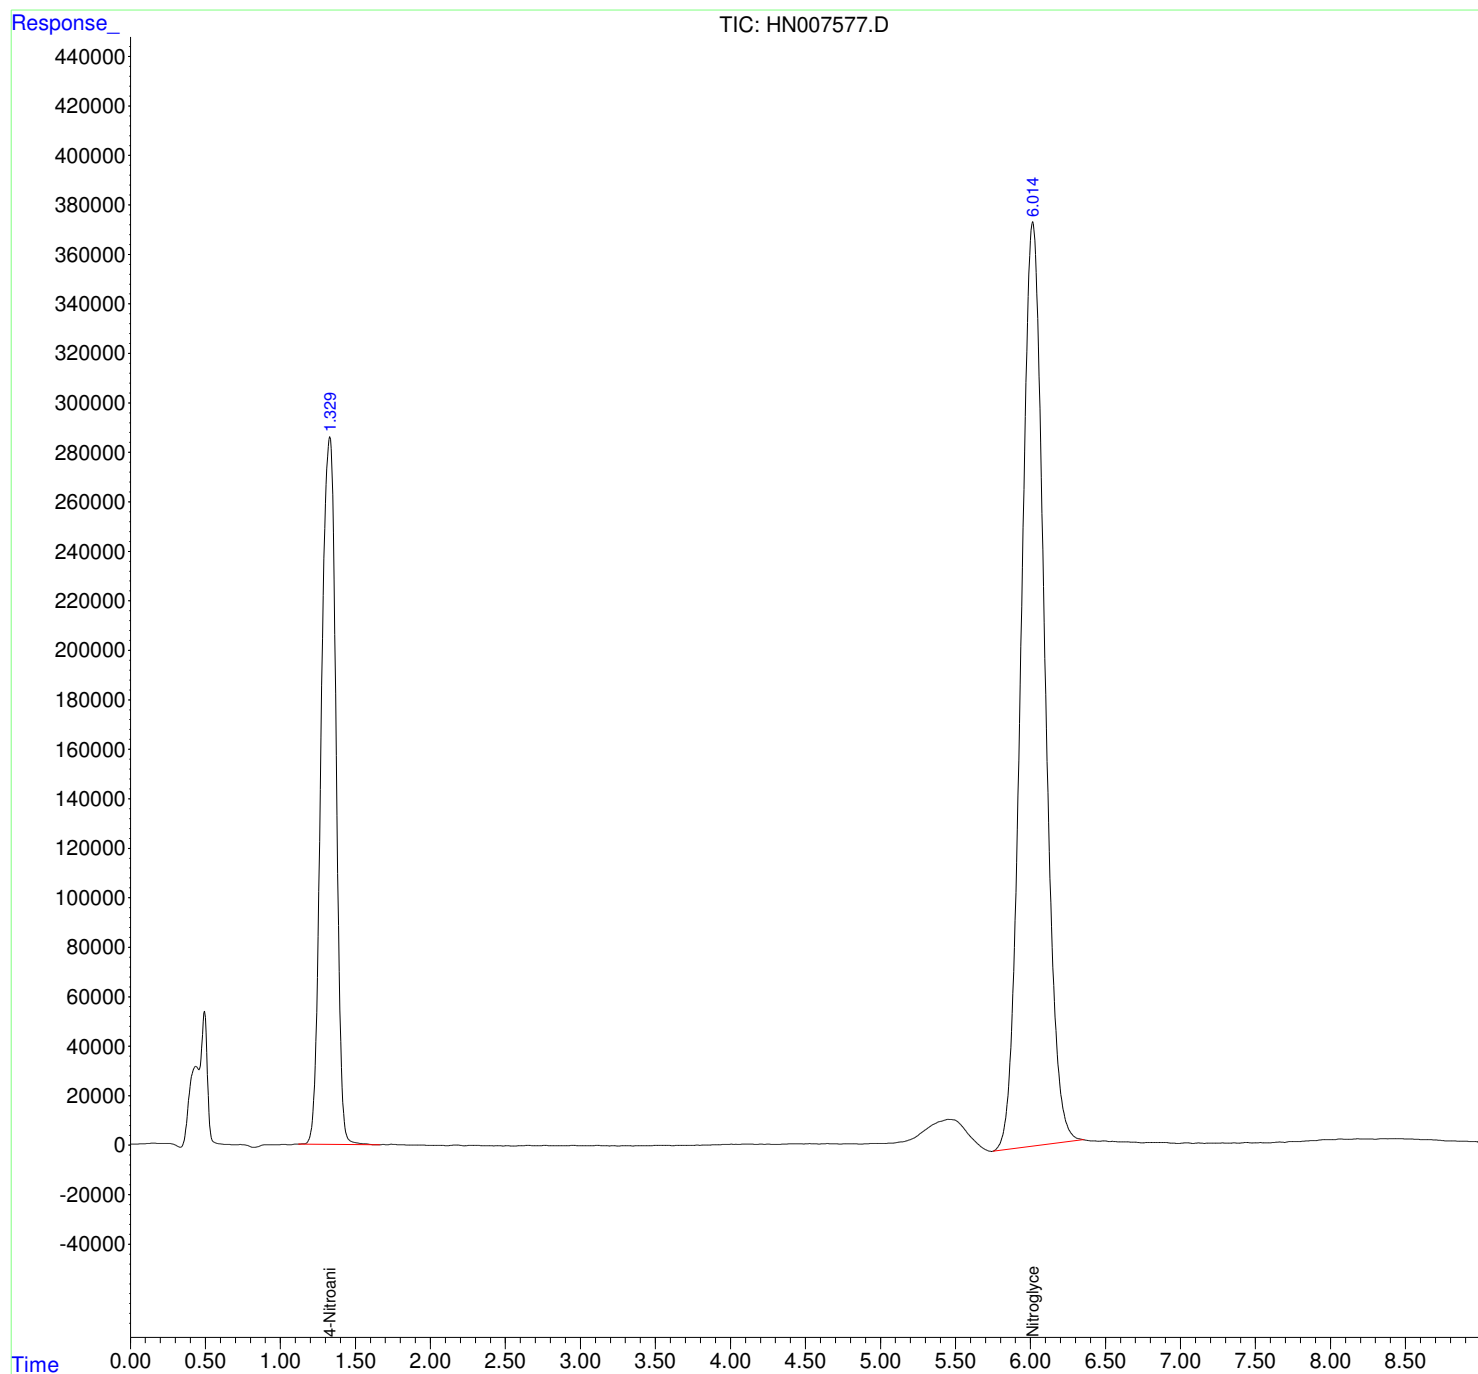


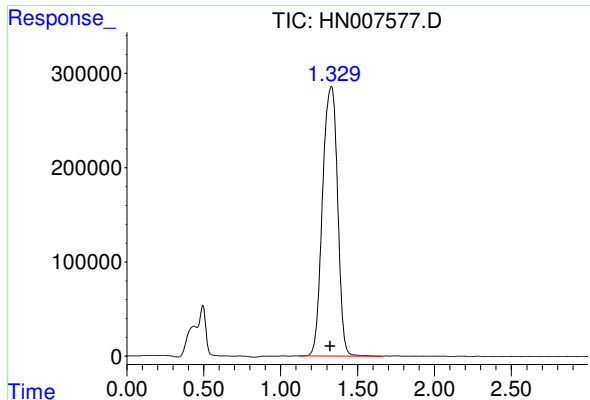

#1 4-Nitroaniline

R.T.: 1.331 min
Delta R.T.: 0.009 min
Response: 19440390
Conc: 4.86 ng/u1

Instrument :
HPLC_N
ClientSampleId :
SSTDICV005

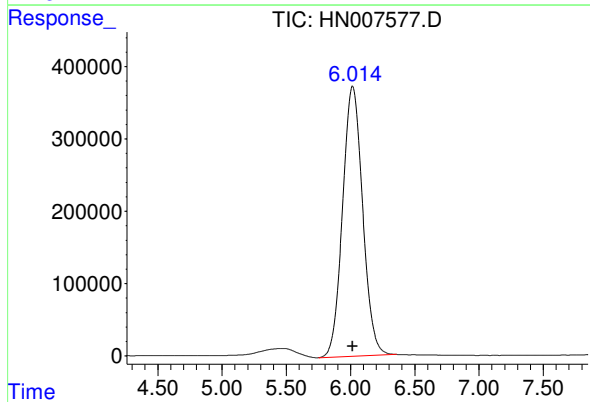

#2 Nitroglycerin

R.T.: 6.016 min
Delta R.T.: 0.002 min
Response: 40534660
Conc: 4.79 ng/u1