

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN101514\
Data File : HN006306.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 15-Oct-2014, 14:15
Operator : HNP
Sample : F4222-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
YS19-GW03-1014

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 16:26:59 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Quant Title :
QLast Update : Mon Mar 09 14:56:25 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.301	1181407	346.739 ug/L
Target Compounds			
2) T HMX	0.929f	367546	81.532 ug/L
3) T RDX	1.705	77159	14.717 ug/L
4) T 1,3,5-Trinitrobenzene	2.659	257504	23.986 ug/L
6) T 3,5-Dinitroaniline	3.880	1110734	95.532 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN101514\
Data File : HN006306.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 15-Oct-2014, 14:15
Operator : HNP
Sample : F4222-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
YS19-GW03-1014

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 16:26:59 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Quant Title :
QLast Update : Mon Mar 09 14:56:25 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

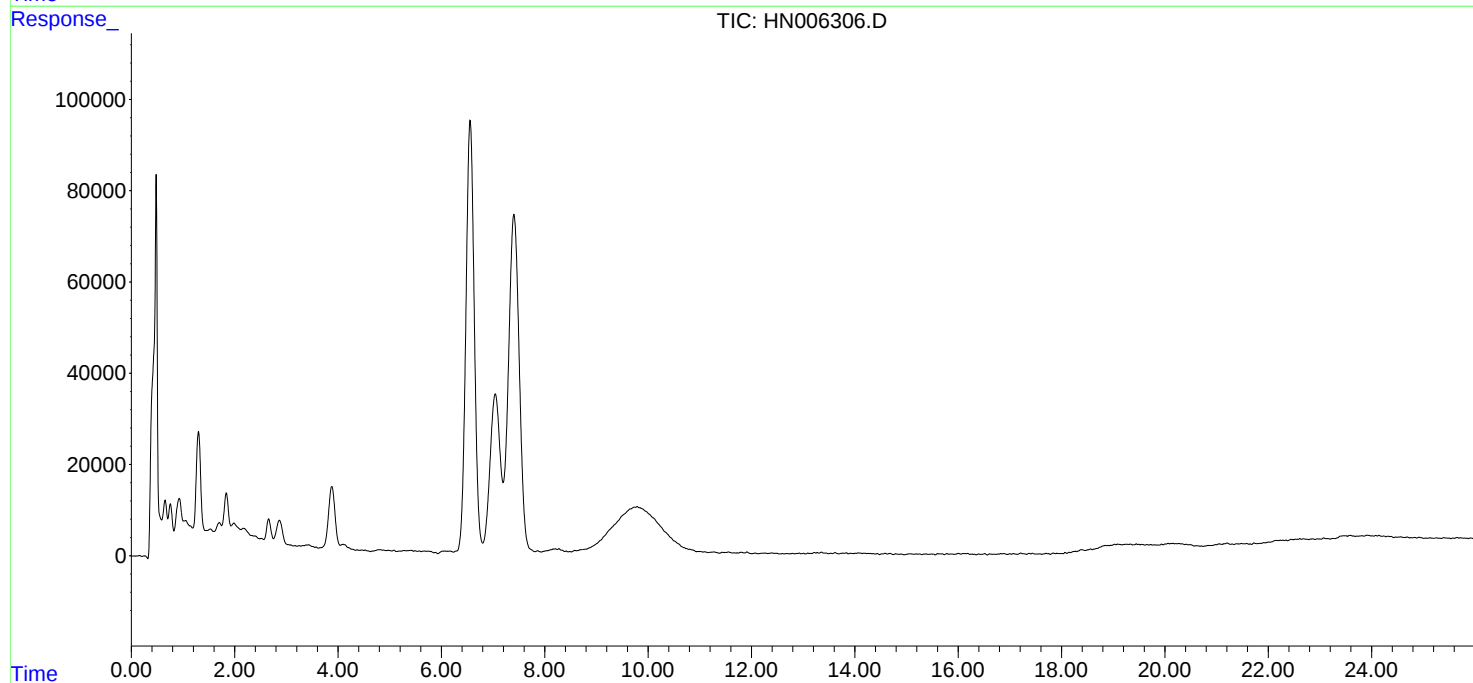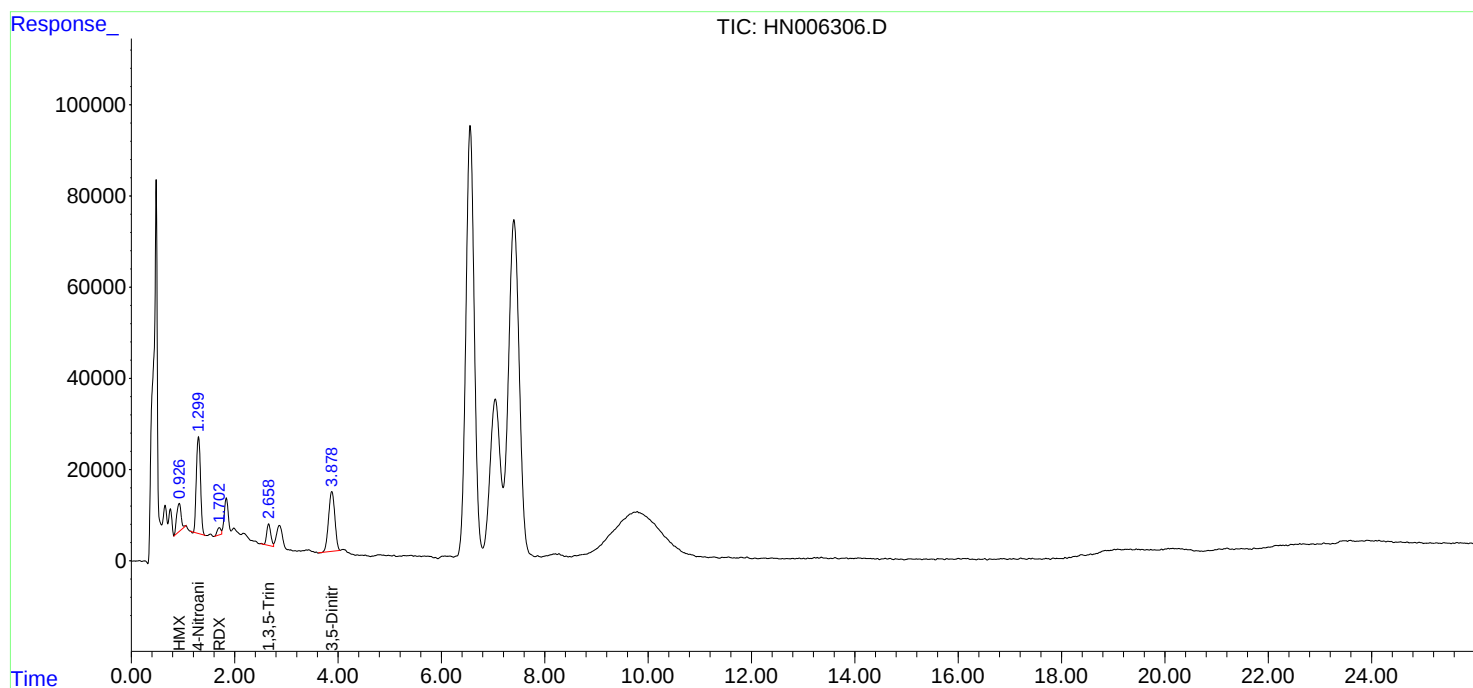


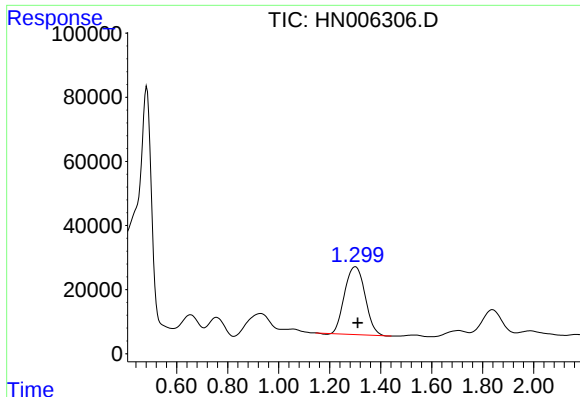

#1 4-Nitroaniline


R.T.: 1.301 min
Delta R.T.: -0.009 min
Response: 1181407
Conc: 346.74 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-GW03-1014

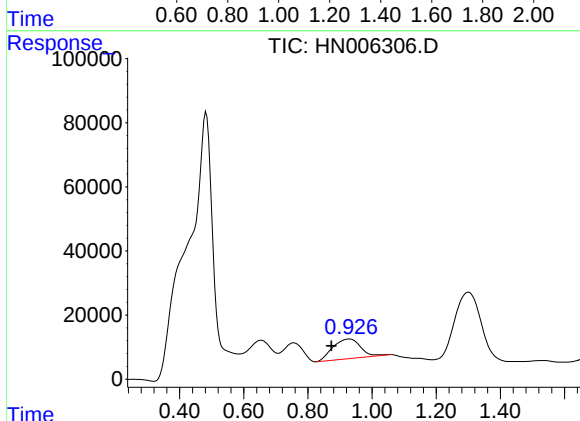


#2 HMX

R.T.: 0.929 min
Delta R.T.: 0.056 min
Response: 367546
Conc: 81.53 ug/L

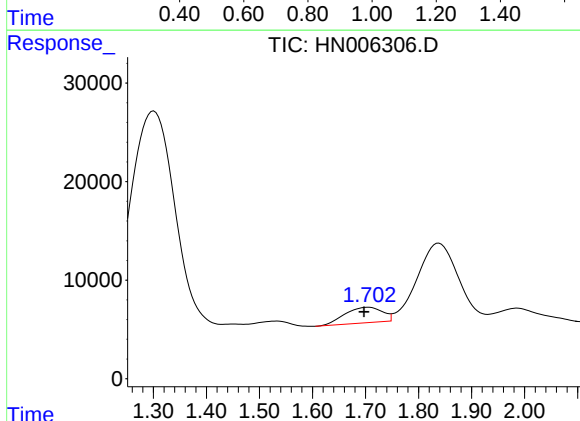


#3 RDX

R.T.: 1.705 min
Delta R.T.: 0.008 min
Response: 77159
Conc: 14.72 ug/L

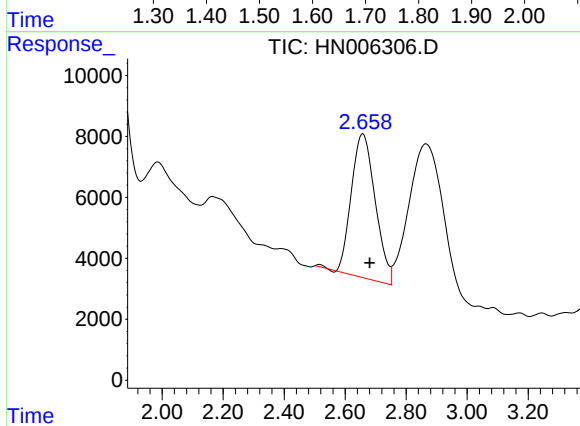

#4 1,3,5-Trinitrobenzene

R.T.: 2.659 min
Delta R.T.: -0.022 min
Response: 257504
Conc: 23.99 ug/L

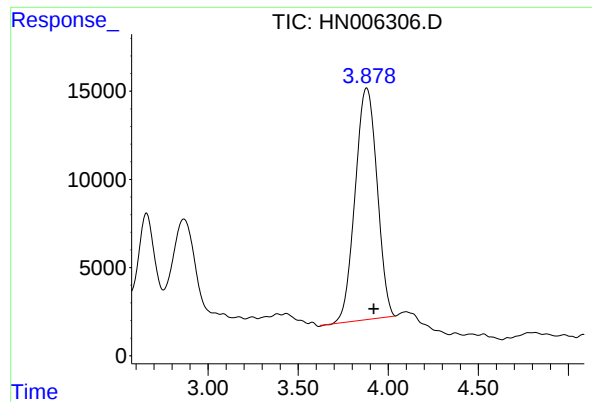

#6 3,5-Dinitroaniline

R.T.: 3.880 min
Delta R.T.: -0.040 min
Response: 1110734
Conc: 95.53 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-GW03-1014