

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN101514\
 Data File : HN006307.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 15-Oct-2014, 14:43
 Operator : HNP
 Sample : F4222-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 YS19-GW03P-1014

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 16:27:07 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
 Quant Title :
 QLast Update : Mon Mar 09 14:56:25 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.302	1194646	350.624 ug/L
Target Compounds			
2) T HMX	0.931f	351256	77.919 ug/L
3) T RDX	1.704	68684	13.100 ug/L
4) T 1,3,5-Trinitrobenzene	2.663	311311	28.998 ug/L
6) T 3,5-Dinitroaniline	3.891	934909	80.410 ug/L
9) T 2,4,6-Trinitrotoluene	6.572f	9211265	839.751 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN101514\
Data File : HN006307.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 15-Oct-2014, 14:43
Operator : HNP
Sample : F4222-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
YS19-GW03P-1014

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 16:27:07 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Quant Title :
QLast Update : Mon Mar 09 14:56:25 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

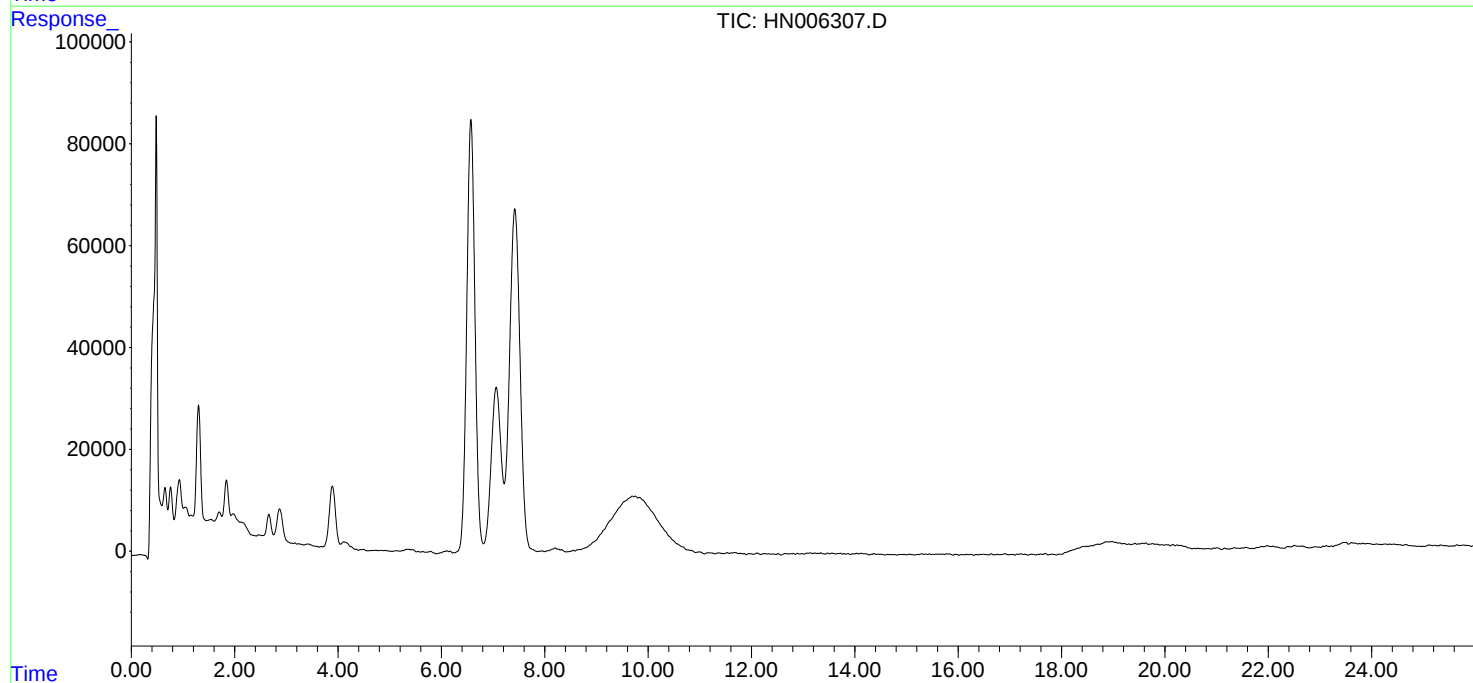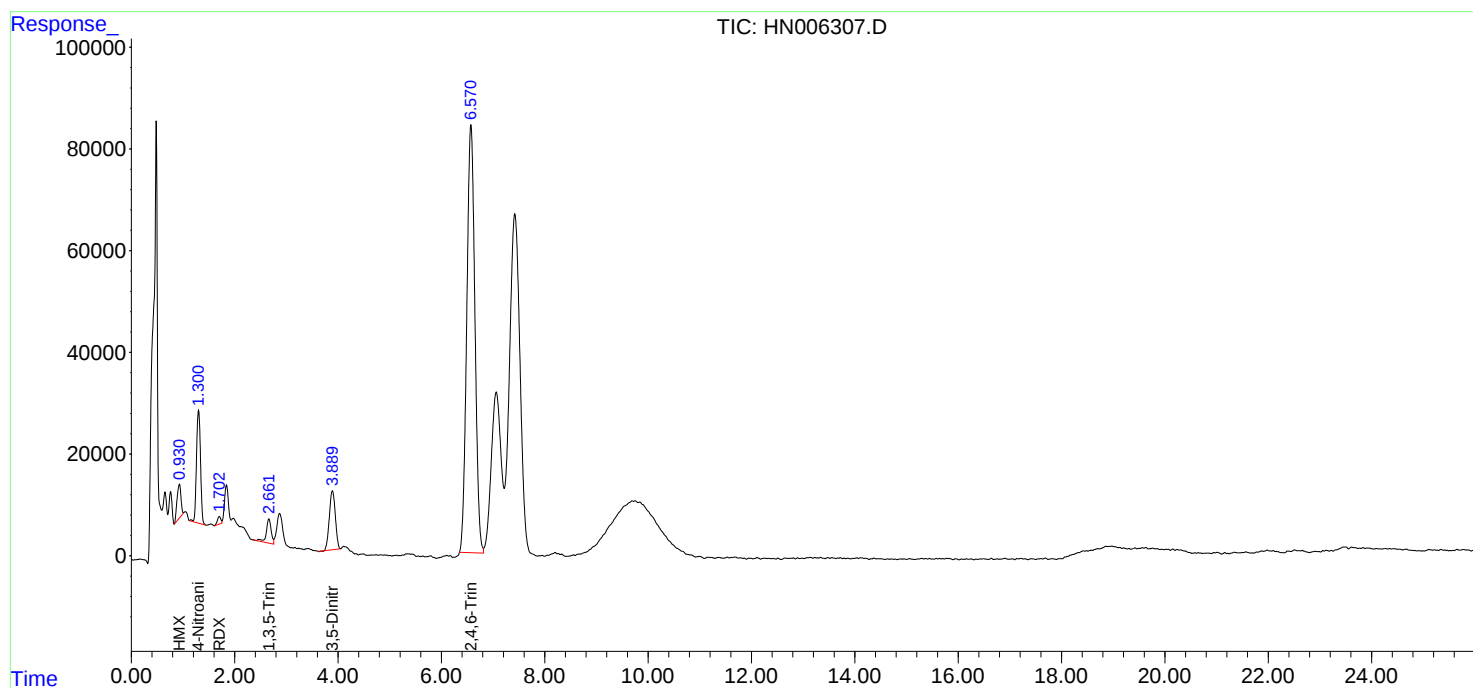


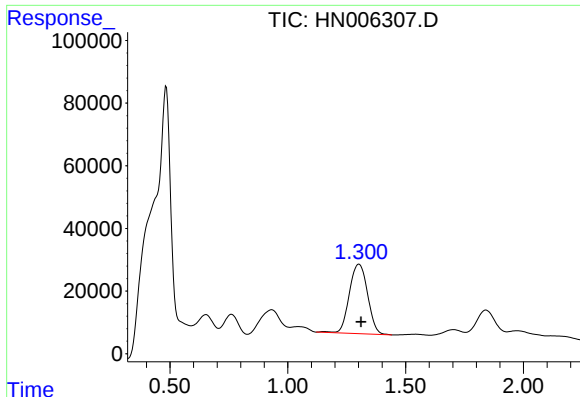

#1 4-Nitroaniline


R.T.: 1.302 min
Delta R.T.: -0.008 min
Response: 1194646
Conc: 350.62 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-GW03P-1014

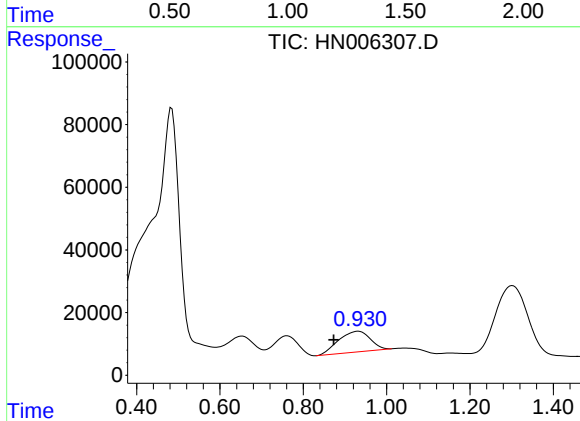


#2 HMX

R.T.: 0.931 min
Delta R.T.: 0.058 min
Response: 351256
Conc: 77.92 ug/L

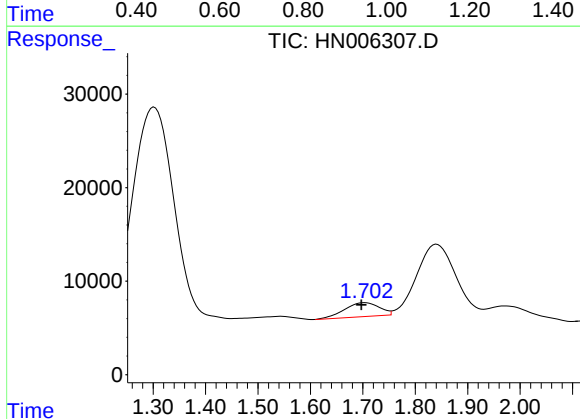


#3 RDX

R.T.: 1.704 min
Delta R.T.: 0.007 min
Response: 68684
Conc: 13.10 ug/L

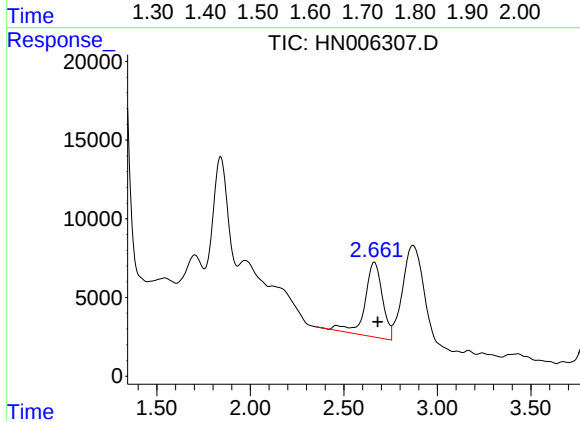

#4 1,3,5-Trinitrobenzene


R.T.: 2.663 min
Delta R.T.: -0.018 min
Response: 311311
Conc: 29.00 ug/L

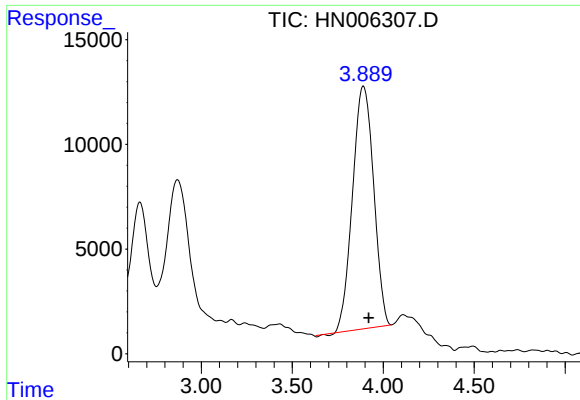

#6 3,5-Dinitroaniline

R.T.: 3.891 min
Delta R.T.: -0.029 min
Response: 934909
Conc: 80.41 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-GW03P-1014

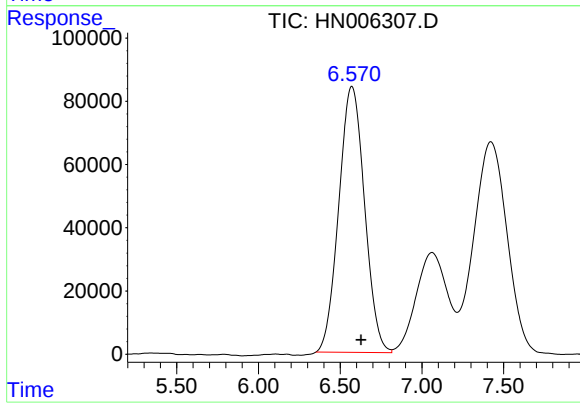

#9 2,4,6-Trinitrotoluene

R.T.: 6.572 min
Delta R.T.: -0.055 min
Response: 9211265
Conc: 839.75 ug/L