

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN101514\
 Data File : HN006311.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 15-Oct-2014, 16:35
 Operator : HNP
 Sample : HSTDCCC0500
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDCCC0500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 16:27:47 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
 Quant Title :
 QLast Update : Mon Mar 09 14:56:25 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.311	1771024	519.789 ug/L
Target Compounds			
2) T HMX	0.871	2042716	453.134 ug/L
3) T RDX	1.694	2776106	529.496 ug/L
4) T 1,3,5-Trinitrobenzene	2.665	5460231	508.613 ug/L
5) T 1,3-Dinitrobenzene	3.545	8199342	502.576 ng/ml
6) T 3,5-Dinitroaniline	3.906	5836917	502.022 ug/L
7) T Nitrobenzene	4.790	4997666	496.258 ug/L
9) T 2,4,6-Trinitrotoluene	6.571f	2441829	222.611 ug/L
13) T 2,6-Dinitrotoluene	8.641f	4057003	487.107 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN101514\
Data File : HN006311.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 15-Oct-2014, 16:35
Operator : HNP
Sample : HSTDCCC0500
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 16:27:47 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Quant Title :
QLast Update : Mon Mar 09 14:56:25 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

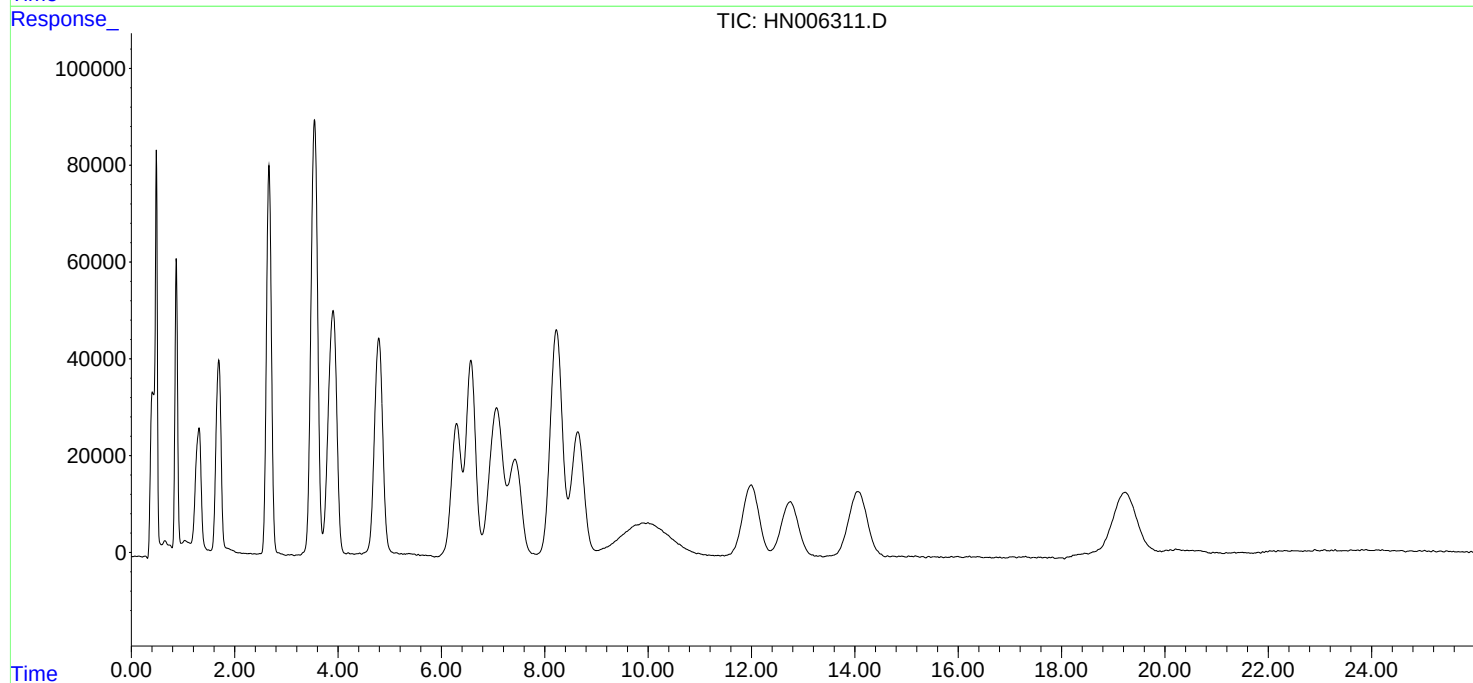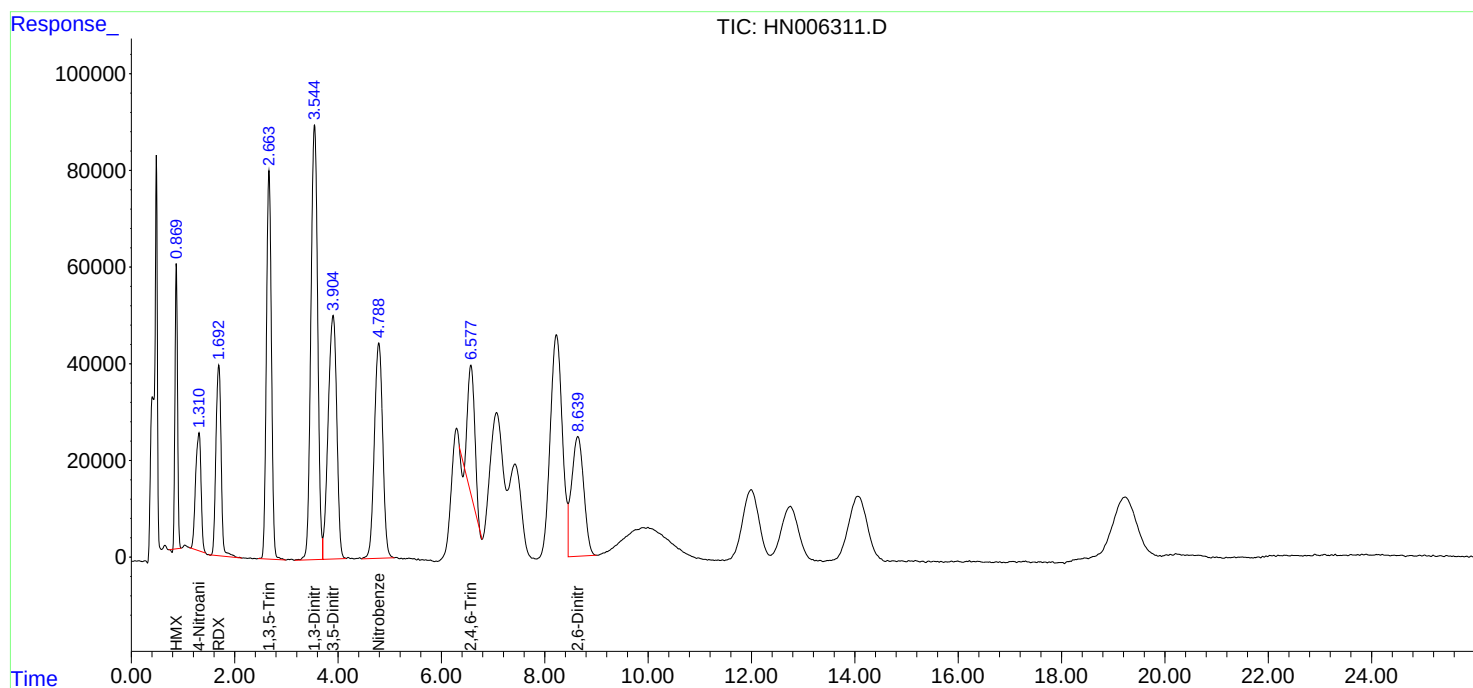


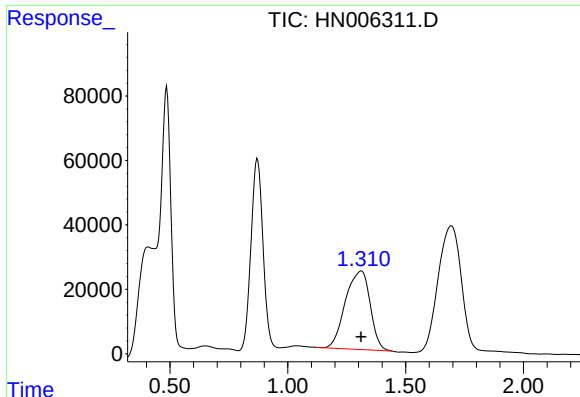

#1 4-Nitroaniline


R.T.: 1.311 min
Delta R.T.: 0.000 min
Response: 1771024
Conc: 519.79 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

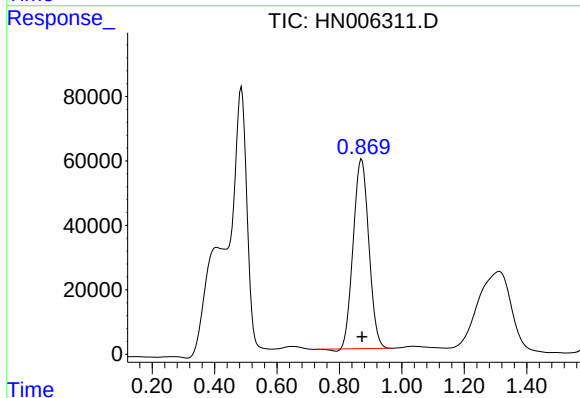


#2 HMX

R.T.: 0.871 min
Delta R.T.: -0.002 min
Response: 2042716
Conc: 453.13 ug/L

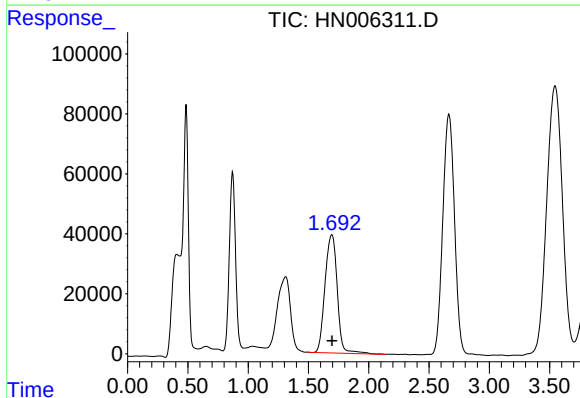


#3 RDX

R.T.: 1.694 min
Delta R.T.: -0.003 min
Response: 2776106
Conc: 529.50 ug/L

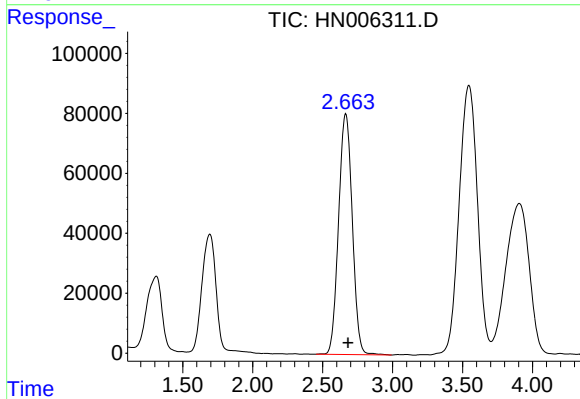

#4 1,3,5-Trinitrobenzene


R.T.: 2.665 min
Delta R.T.: -0.016 min
Response: 5460231
Conc: 508.61 ug/L

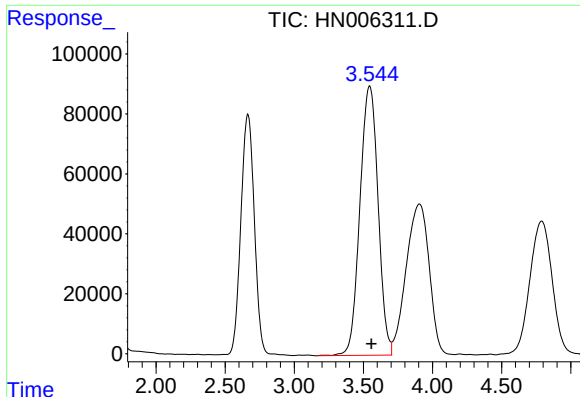

#5 1,3-Dinitrobenzene


R.T.: 3.545 min
Delta R.T.: -0.012 min
Response: 8199342
Conc: 502.58 ng/ml

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

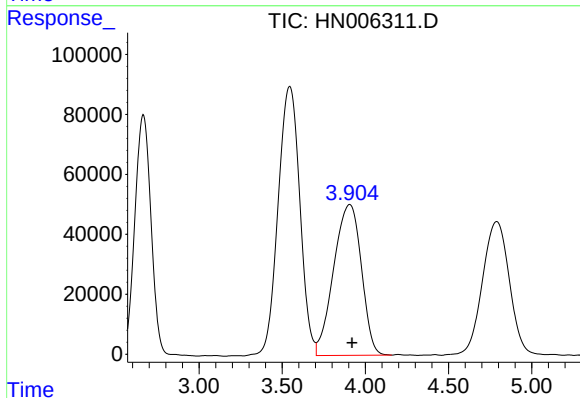


#6 3,5-Dinitroaniline

R.T.: 3.906 min
Delta R.T.: -0.014 min
Response: 5836917
Conc: 502.02 ug/L

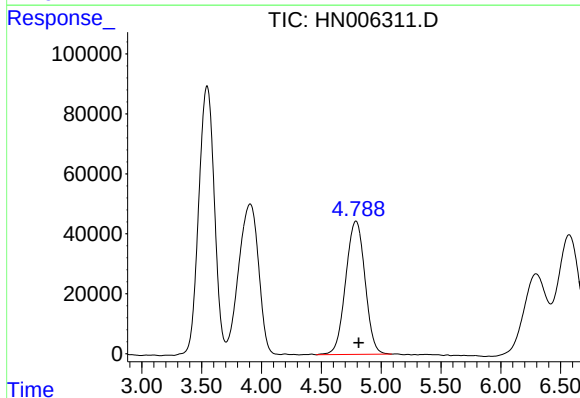


#7 Nitrobenzene

R.T.: 4.790 min
Delta R.T.: -0.024 min
Response: 4997666
Conc: 496.26 ug/L

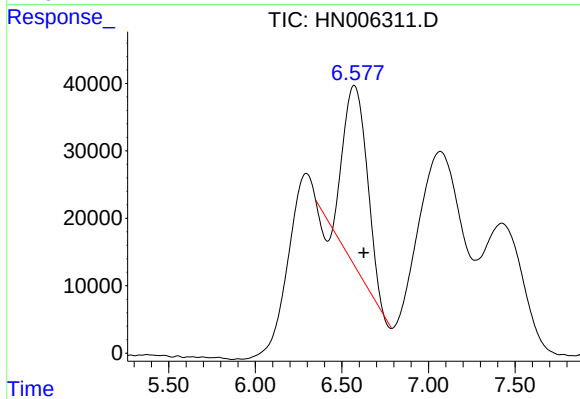

#9 2,4,6-Trinitrotoluene

R.T.: 6.571 min
Delta R.T.: -0.056 min
Response: 2441829
Conc: 222.61 ug/L

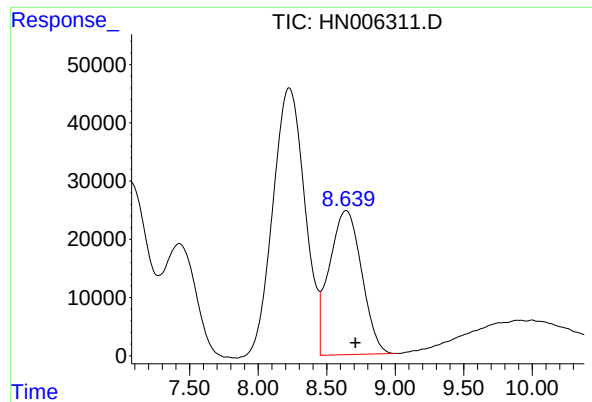

#13 2,6-Dinitrotoluene

R.T.: 8.641 min
Delta R.T.: -0.070 min
Response: 4057003
Conc: 487.11 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500