

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN101514\
 Data File : HN006333.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 16-Oct-2014, 02:51
 Operator : HNP
 Sample : HSTDCCC0500
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDCCC0500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 16:30:33 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
 Quant Title :
 QLast Update : Mon Mar 09 14:56:25 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.308	1680993	493.365 ug/L
Target Compounds			
2) T HMX	0.871	2044079	453.436 ug/L
3) T RDX	1.690	2688987	512.880 ug/L
4) T 1,3,5-Trinitrobenzene	2.656	5445571	507.248 ug/L
5) T 1,3-Dinitrobenzene	3.529	8255914	506.044 ng/ml
6) T 3,5-Dinitroaniline	3.879	5931511	510.158 ug/L
7) T Nitrobenzene	4.776	5068903	503.331 ug/L
9) T 2,4,6-Trinitrotoluene	6.564f	2667953	243.226 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN101514\
Data File : HN006333.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 16-Oct-2014, 02:51
Operator : HNP
Sample : HSTDCCC0500
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 16:30:33 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Quant Title :
QLast Update : Mon Mar 09 14:56:25 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

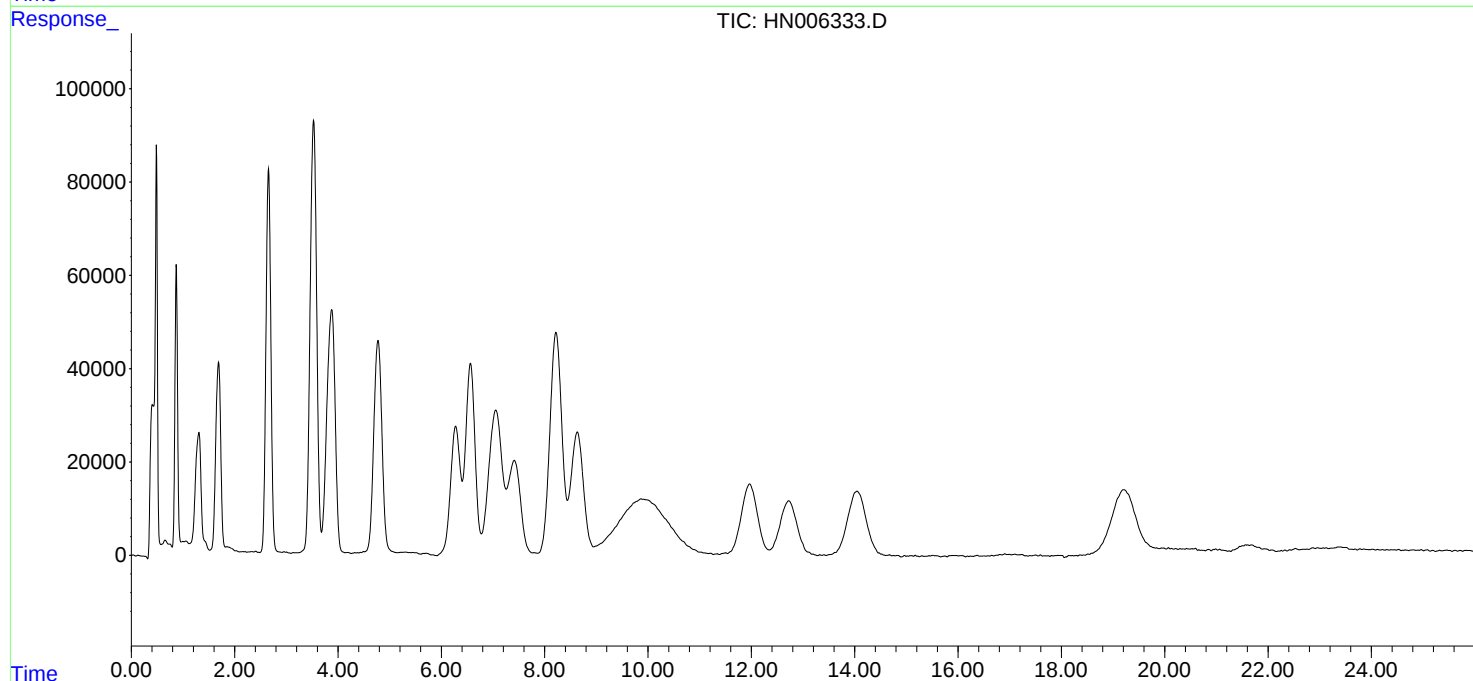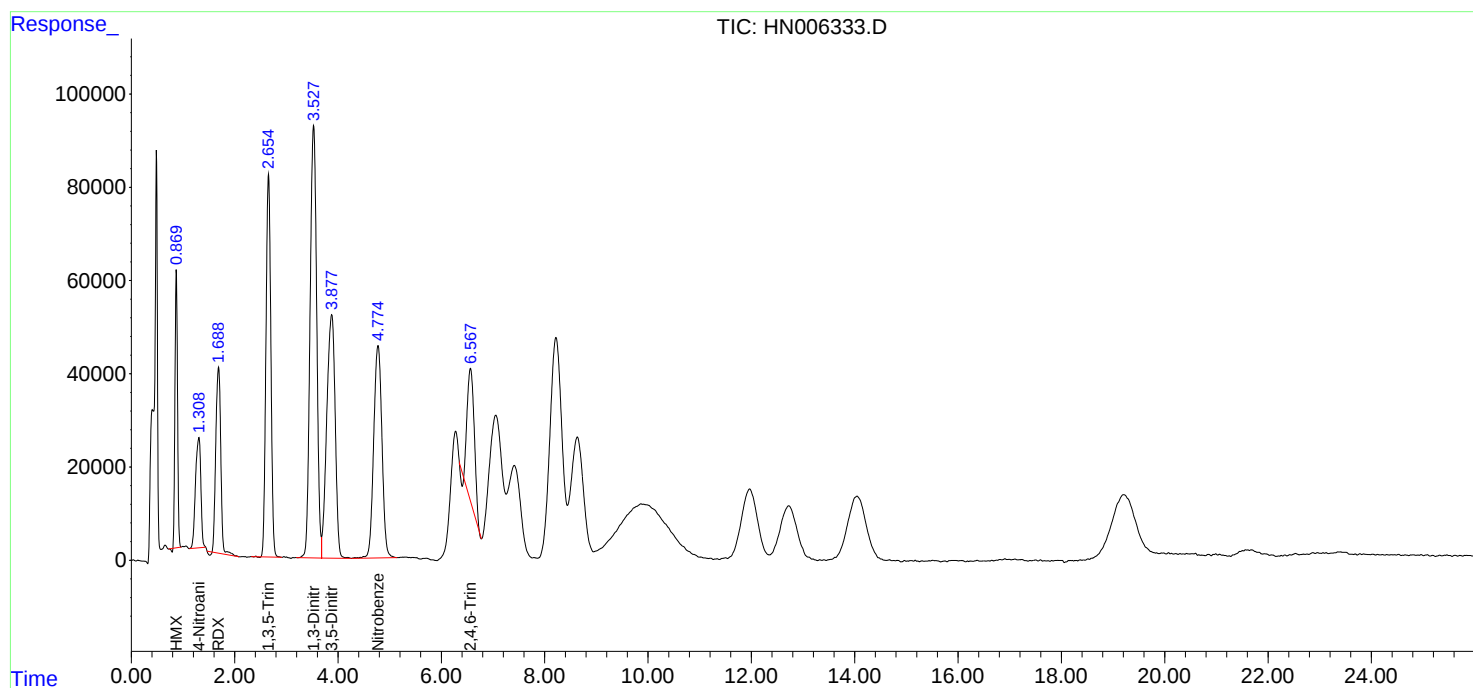


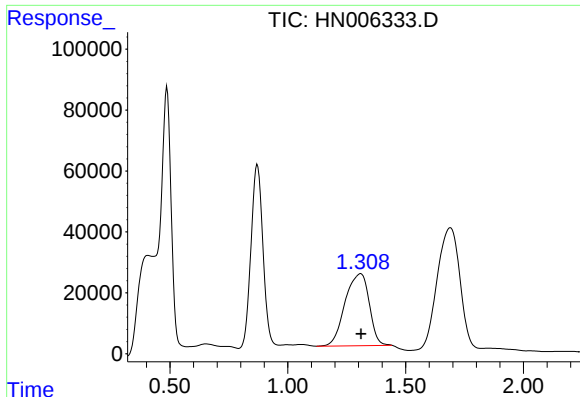

#1 4-Nitroaniline


R.T.: 1.308 min
Delta R.T.: -0.002 min
Response: 1680993
Conc: 493.37 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

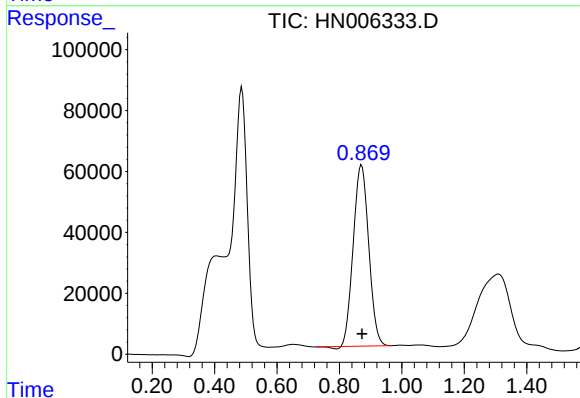


#2 HMX

R.T.: 0.871 min
Delta R.T.: -0.002 min
Response: 2044079
Conc: 453.44 ug/L

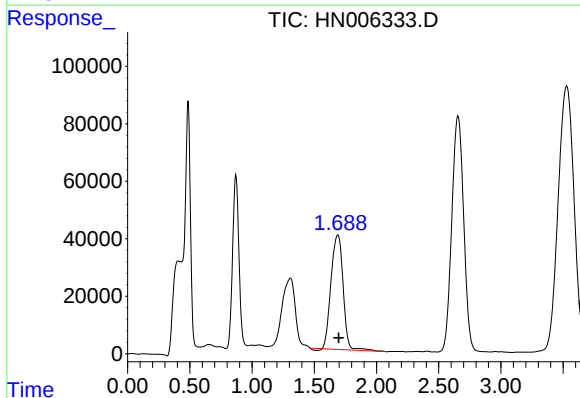


#3 RDX

R.T.: 1.690 min
Delta R.T.: -0.007 min
Response: 2688987
Conc: 512.88 ug/L

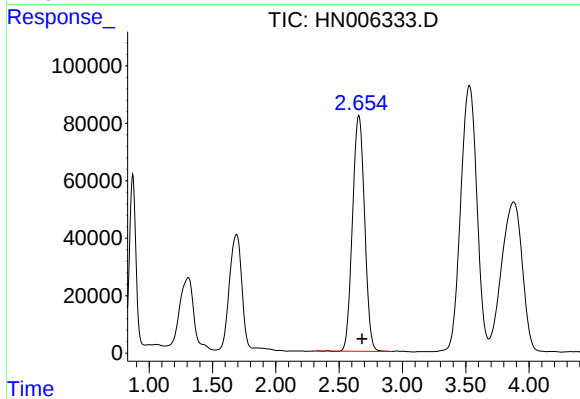

#4 1,3,5-Trinitrobenzene


R.T.: 2.656 min
Delta R.T.: -0.025 min
Response: 5445571
Conc: 507.25 ug/L

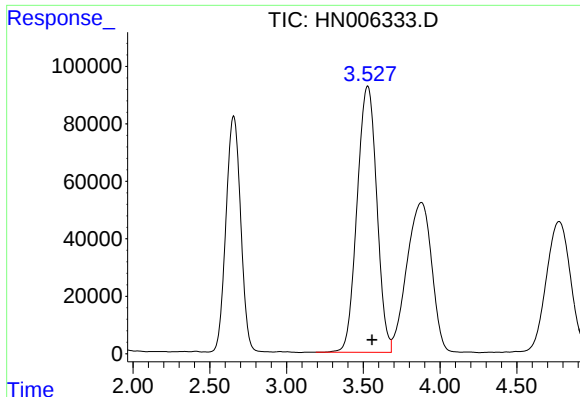

#5 1,3-Dinitrobenzene


R.T.: 3.529 min
Delta R.T.: -0.029 min
Response: 8255914
Conc: 506.04 ng/ml

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

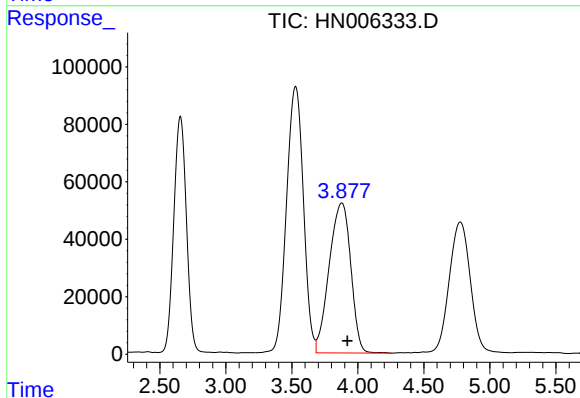


#6 3,5-Dinitroaniline

R.T.: 3.879 min
Delta R.T.: -0.042 min
Response: 5931511
Conc: 510.16 ug/L

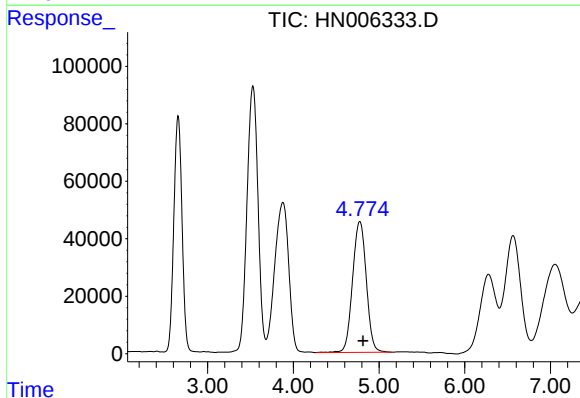

#7 Nitrobenzene

R.T.: 4.776 min
Delta R.T.: -0.038 min
Response: 5068903
Conc: 503.33 ug/L

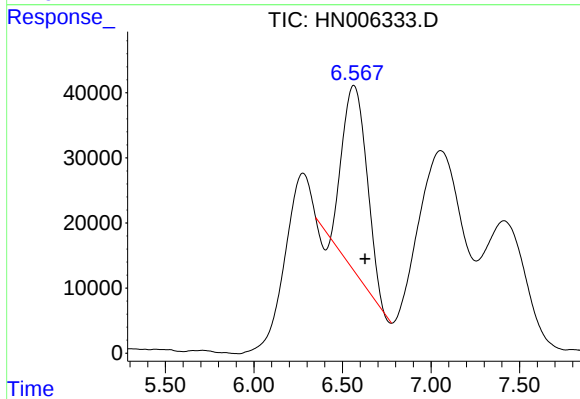

#9 2,4,6-Trinitrotoluene

R.T.: 6.564 min
Delta R.T.: -0.063 min
Response: 2667953
Conc: 243.23 ug/L