

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN101514\
 Data File : HN006342.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 16-Oct-2014, 07:03
 Operator : HNP
 Sample : F4204-05MSD
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 YS19-SB50-02-03-1014MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 16:31:36 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
 Quant Title :
 QLast Update : Mon Mar 09 14:56:25 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.327	572019	167.885 ug/L
Target Compounds			
2) T HMX	0.888	514009	114.022 ug/L
3) T RDX	1.711	632409	120.622 ug/L
4) T 1,3,5-Trinitrobenzene	2.712	1281532	119.373 ug/L
5) T 1,3-Dinitrobenzene	3.608f	1990408	122.001 ng/ml
6) T 3,5-Dinitroaniline	3.966	1467590	126.224 ug/L
7) T Nitrobenzene	4.882f	1181293	117.300 ug/L
8) T Tetryl	6.413f	157255	24.274 ug/L
10) T 2-Amino-4,6-dinitroto...	7.205f	1204843	104.658 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN101514\
Data File : HN006342.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 16-Oct-2014, 07:03
Operator : HNP
Sample : F4204-05MSD
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
YS19-SB50-02-03-1014MSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 16:31:36 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Quant Title :
QLast Update : Mon Mar 09 14:56:25 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

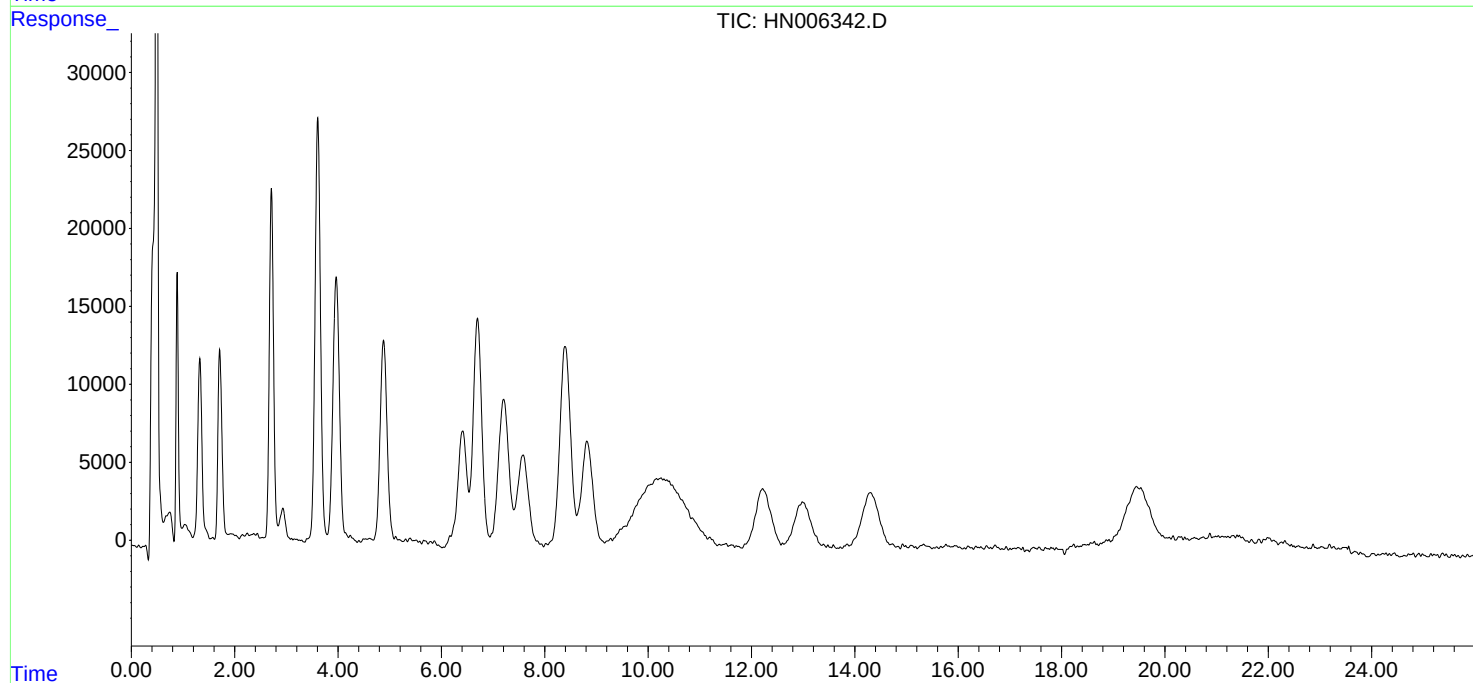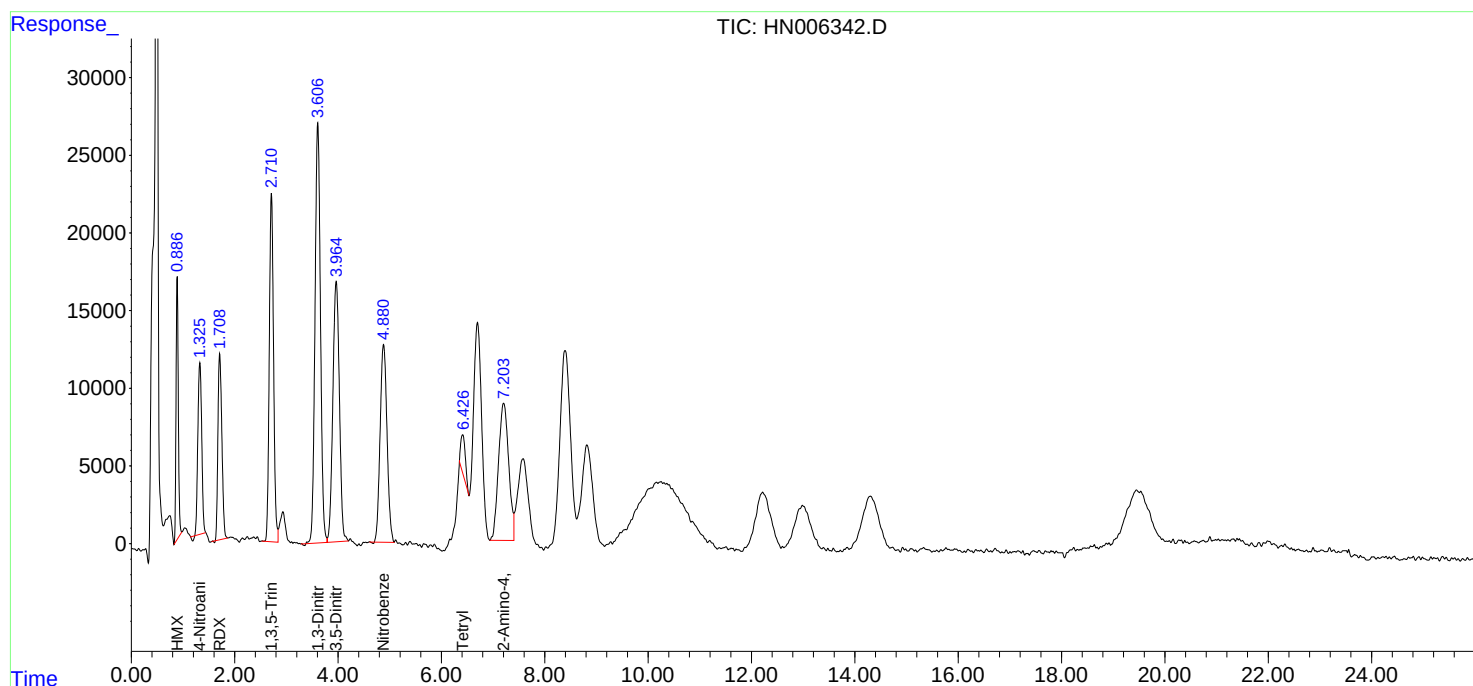


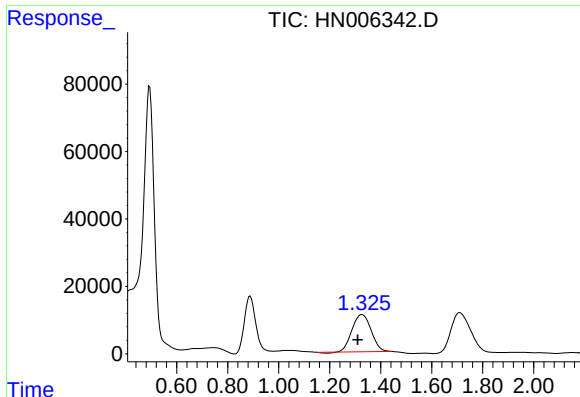

#1 4-Nitroaniline


R.T.: 1.327 min
Delta R.T.: 0.017 min
Response: 572019
Conc: 167.89 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-SB50-02-03-1014MSD

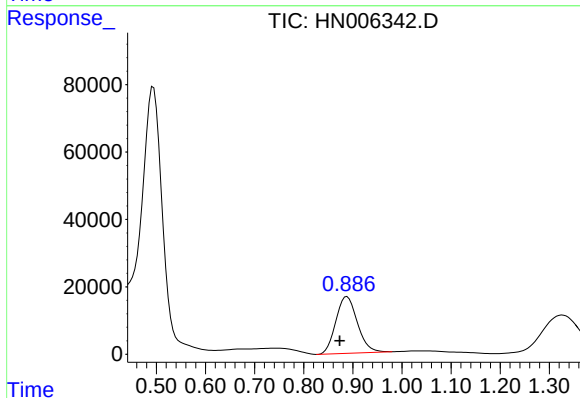


#2 HMX

R.T.: 0.888 min
Delta R.T.: 0.015 min
Response: 514009
Conc: 114.02 ug/L

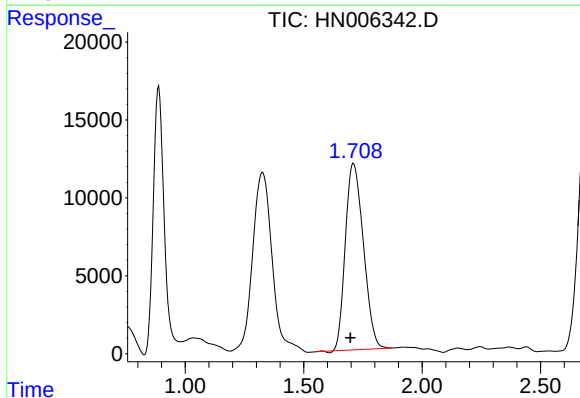


#3 RDX

R.T.: 1.711 min
Delta R.T.: 0.014 min
Response: 632409
Conc: 120.62 ug/L

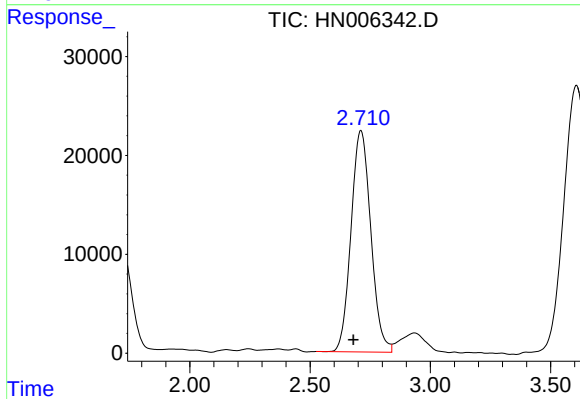

#4 1,3,5-Trinitrobenzene


R.T.: 2.712 min
Delta R.T.: 0.031 min
Response: 1281532
Conc: 119.37 ug/L

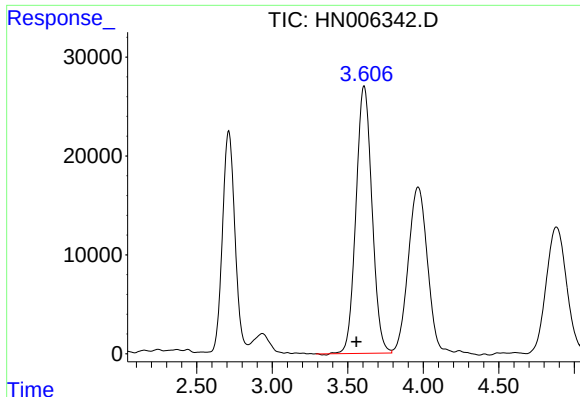

#5 1,3-Dinitrobenzene


R.T.: 3.608 min
Delta R.T.: 0.051 min
Response: 1990408
Conc: 122.00 ng/ml

Instrument :
HPLC_N
ClientSampleId :
YS19-SB50-02-03-1014MSD

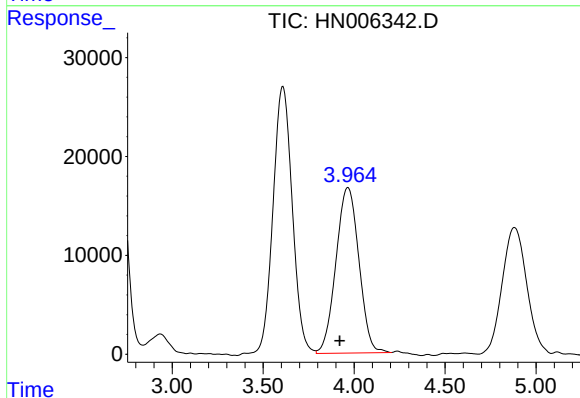


#6 3,5-Dinitroaniline

R.T.: 3.966 min
Delta R.T.: 0.046 min
Response: 1467590
Conc: 126.22 ug/L

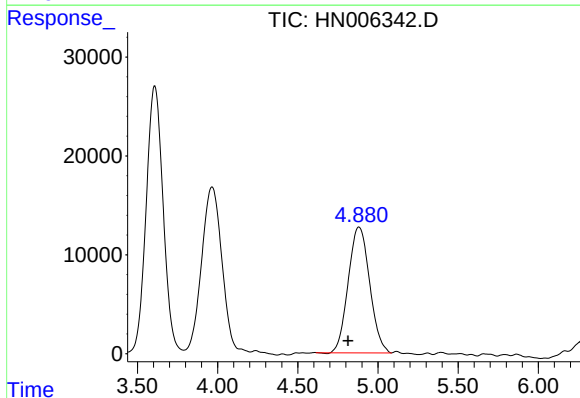


#7 Nitrobenzene

R.T.: 4.882 min
Delta R.T.: 0.068 min
Response: 1181293
Conc: 117.30 ug/L

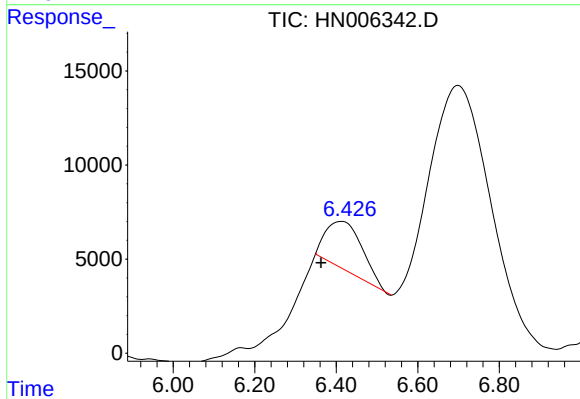

#8 Tetryl

R.T.: 6.413 min
Delta R.T.: 0.051 min
Response: 157255
Conc: 24.27 ug/L

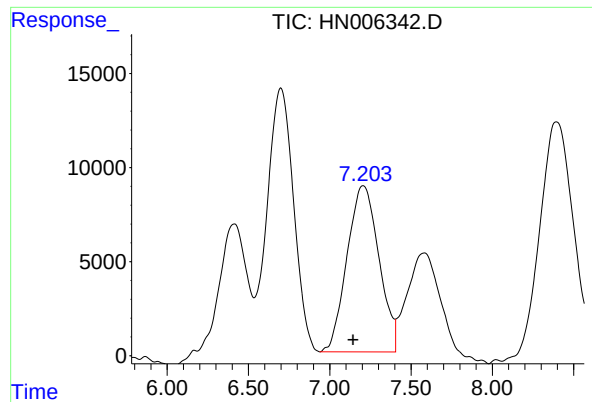

#10 2-Amino-4,6-dinitrotoluene

R.T.: 7.205 min
Delta R.T.: 0.062 min
Response: 1204843
Conc: 104.66 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-SB50-02-03-1014MSD