

Data Path : Z:\HPCHEM1\HPLC\_N\Data\HN101514\  
Data File : HN006343.D  
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
Acq On : 16-Oct-2014, 07:32  
Operator : HNP  
Sample : F4204-06  
Misc :  
ALS Vial : 41 Sample Multiplier: 1

Instrument :  
HPLC\_N  
ClientSampleId :  
YS19-SB51-02-03-1014

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 10 16:31:44 2015  
Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN100214.M  
Quant Title :  
QLast Update : Mon Mar 09 14:56:25 2015  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

| Compound                    | R.T.  | Response | Conc Units   |
|-----------------------------|-------|----------|--------------|
| -----                       |       |          |              |
| System Monitoring Compounds |       |          |              |
| 1) S 4-Nitroaniline         | 1.304 | 602833   | 176.929 ug/L |
| Target Compounds            |       |          |              |
| -----                       |       |          |              |

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC\_N\Data\HN101514\  
Data File : HN006343.D  
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
Acq On : 16-Oct-2014, 07:32  
Operator : HNP  
Sample : F4204-06  
Misc :  
ALS Vial : 41 Sample Multiplier: 1

Instrument :  
HPLC\_N  
ClientSampleId :  
YS19-SB51-02-03-1014

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 10 16:31:44 2015  
Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN100214.M  
Quant Title :  
QLast Update : Mon Mar 09 14:56:25 2015  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

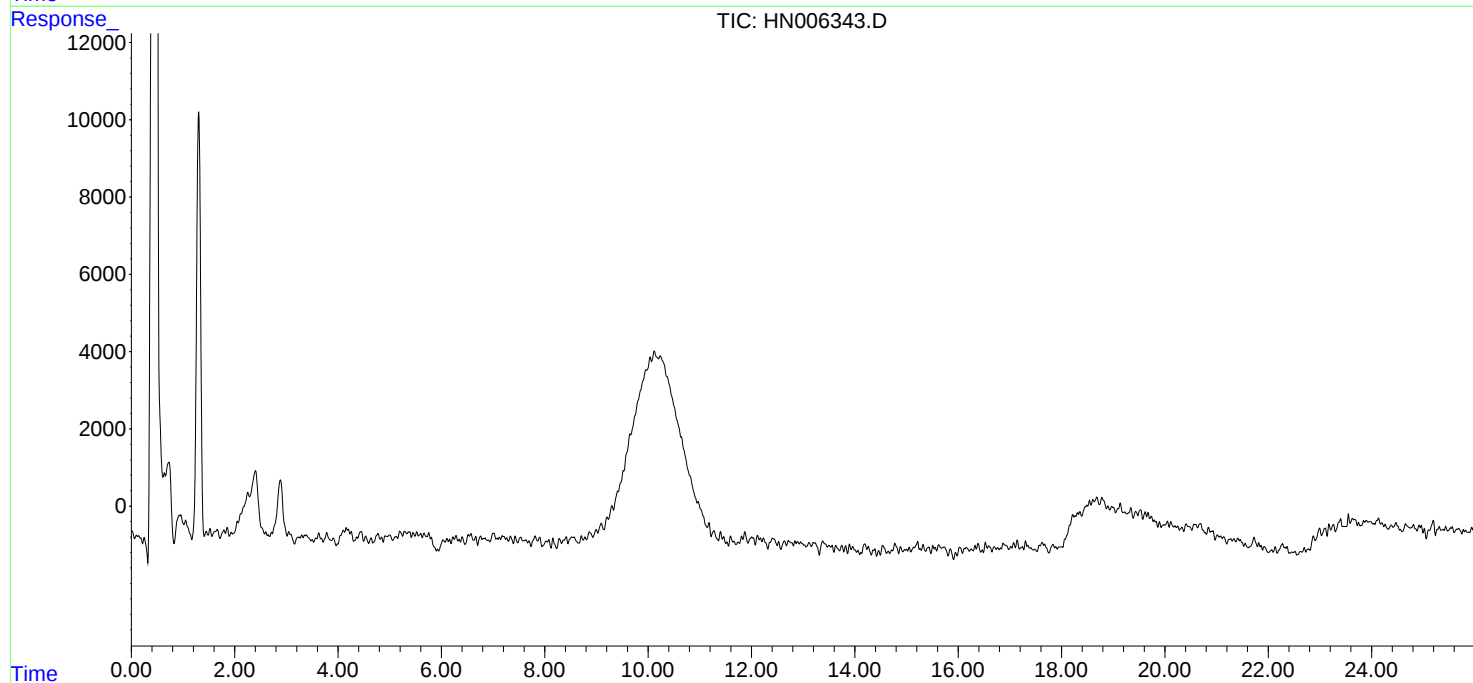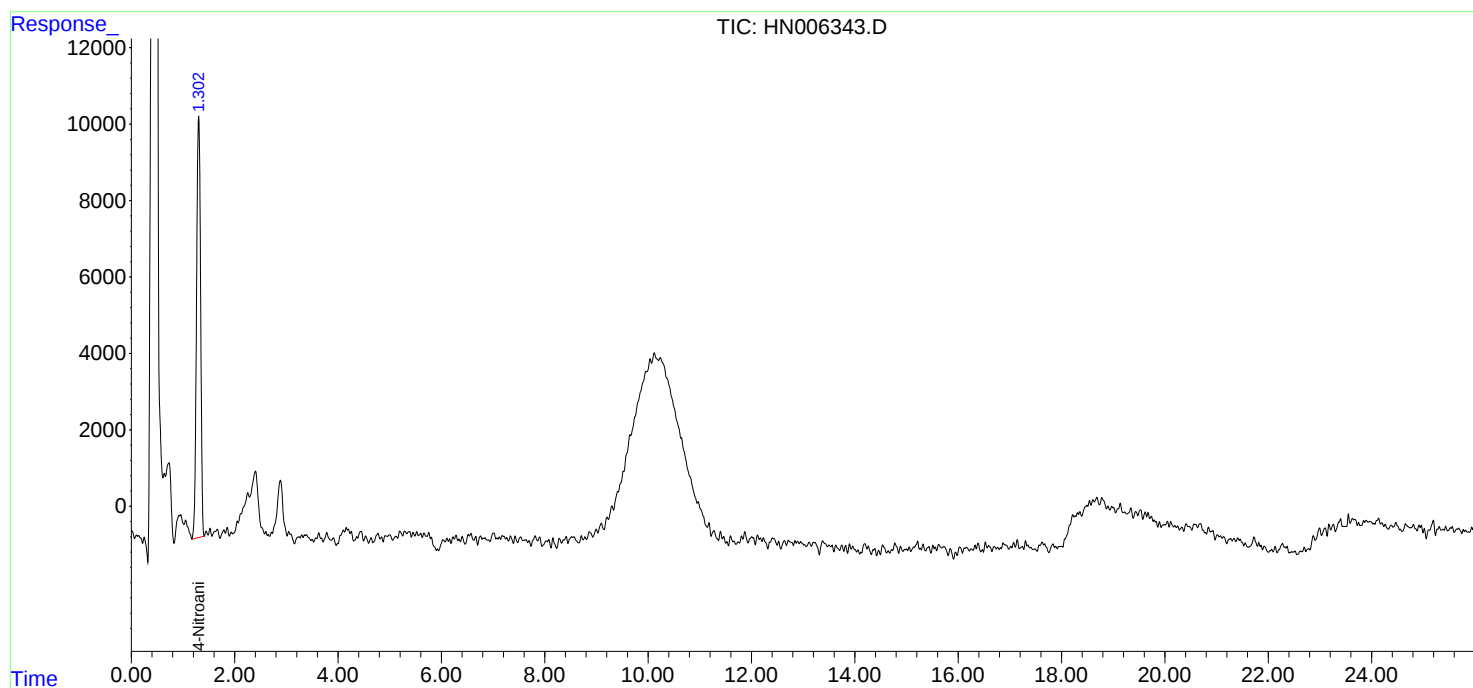

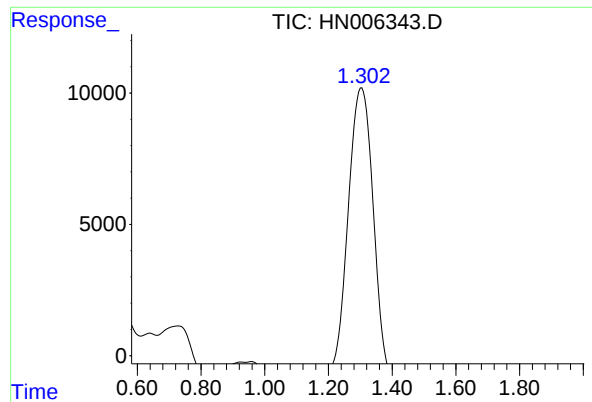

#1 4-Nitroaniline

R.T.: 1.304 min  
Delta R.T.: -0.006 min  
Response: 602833  
Conc: 176.93 ug/L

Instrument :  
HPLC\_N  
ClientSampleId :  
YS19-SB51-02-03-1014