

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN101514\
 Data File : HN006307.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 15-Oct-2014, 14:43
 Operator : HNP
 Sample : F4222-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 YS19-GW03P-1014

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 15:17:44 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
 Quant Title :
 QLast Update : Wed Mar 04 13:53:50 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.302	1161949	341.028 ug/L
Target Compounds			
6) T 3,5-Dinitroaniline	3.891	927329	79.758 ug/L
9) T 2,4,6-Trinitrotoluene	6.572	9456367	862.096 ug/L
10) T 2-Amino-4,6-dinitroto...	7.062	4344971	377.425 ug/L
11) T 4-Amino-2,6-dinitroto...	7.422	9627332	1572.470 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN101514\
Data File : HN006307.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 15-Oct-2014, 14:43
Operator : HNP
Sample : F4222-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
YS19-GW03P-1014

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 15:17:44 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Quant Title :
QLast Update : Wed Mar 04 13:53:50 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

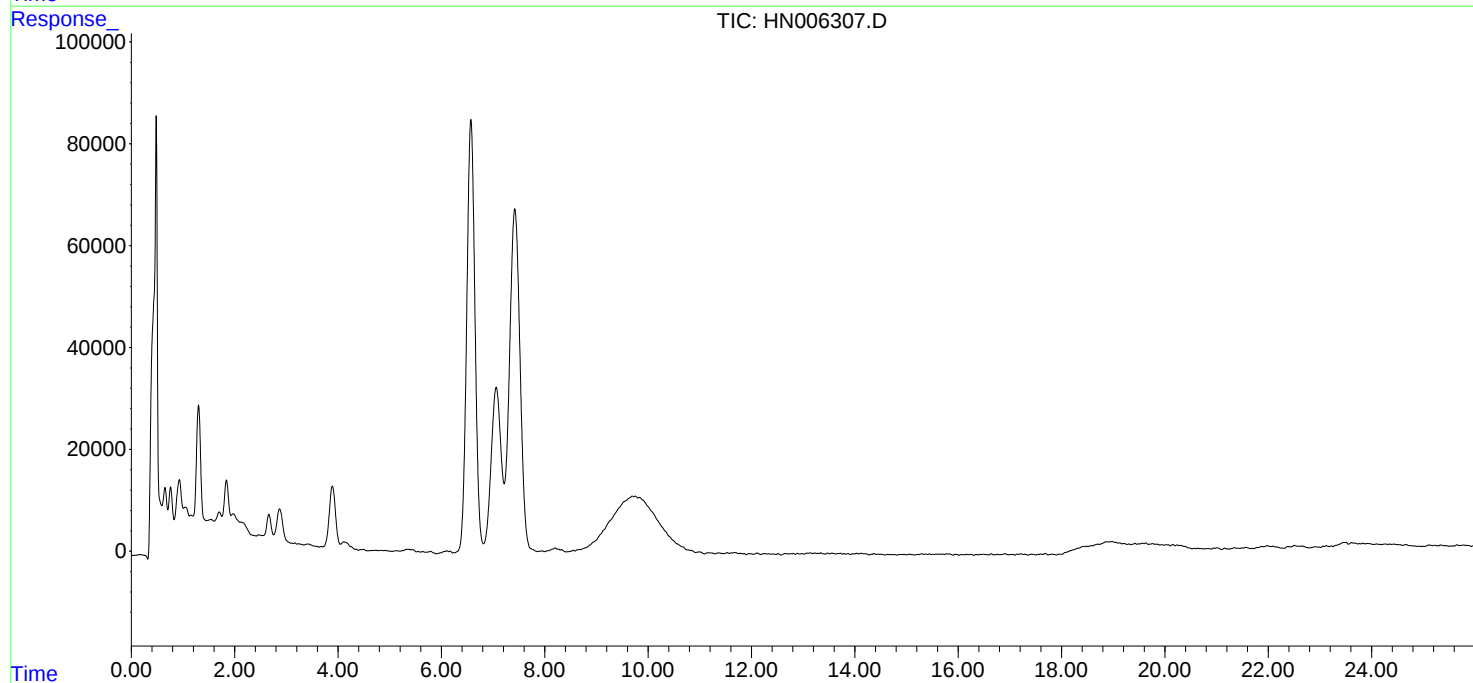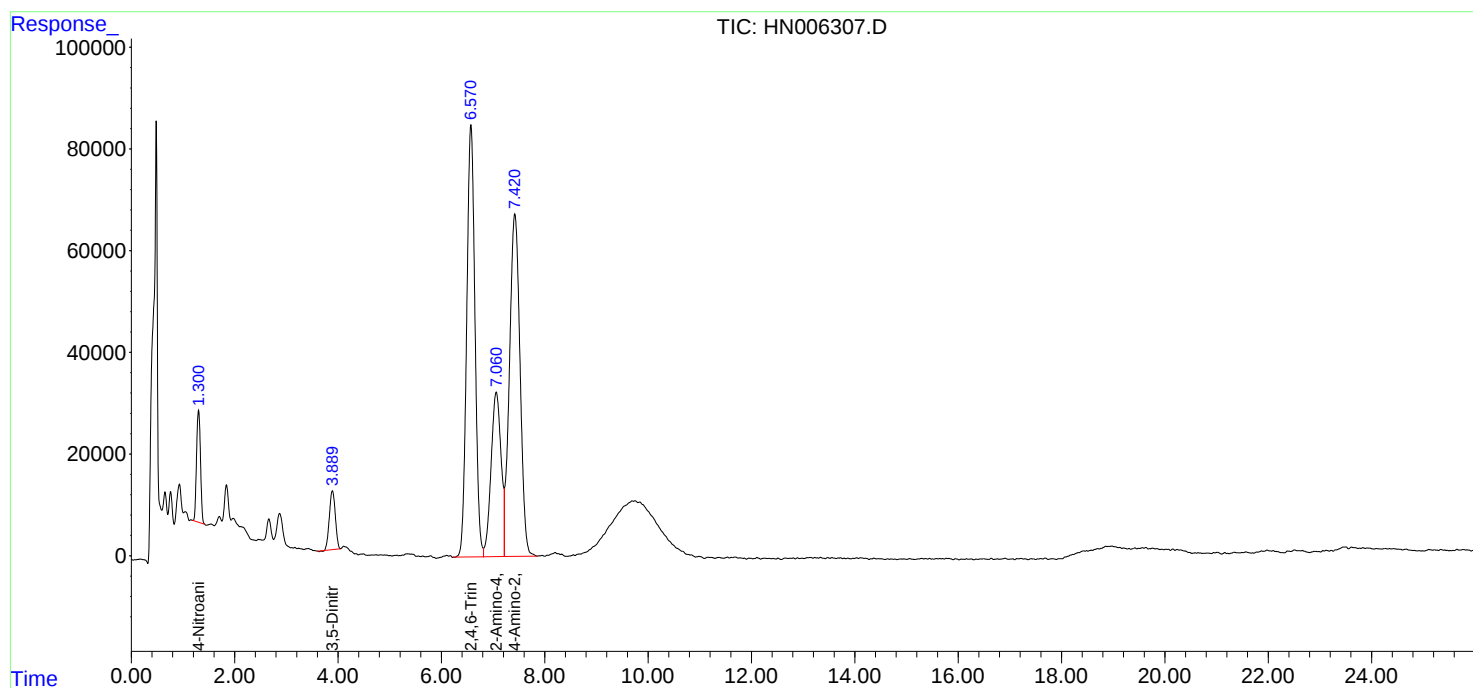


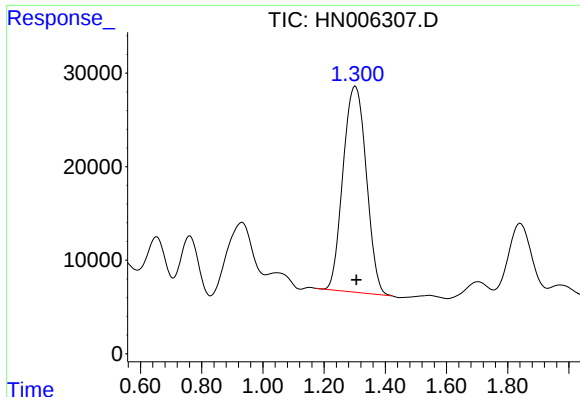

#1 4-Nitroaniline


R.T.: 1.302 min
Delta R.T.: -0.003 min
Response: 1161949
Conc: 341.03 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-GW03P-1014

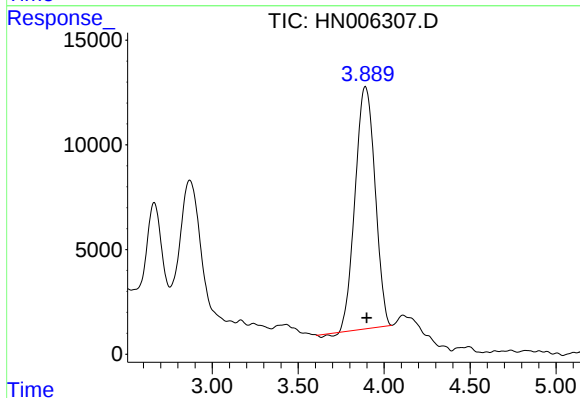


#6 3,5-Dinitroaniline

R.T.: 3.891 min
Delta R.T.: -0.009 min
Response: 927329
Conc: 79.76 ug/L

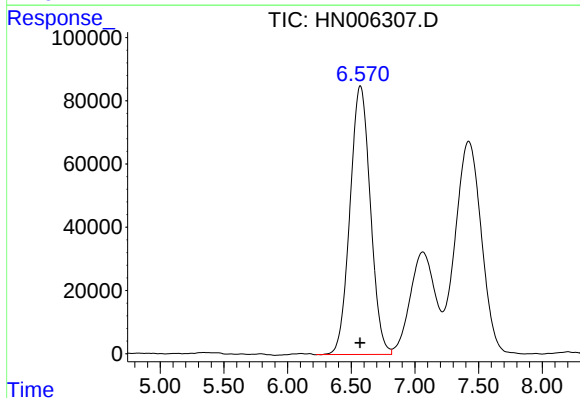


#9 2,4,6-Trinitrotoluene

R.T.: 6.572 min
Delta R.T.: 0.003 min
Response: 9456367
Conc: 862.10 ug/L

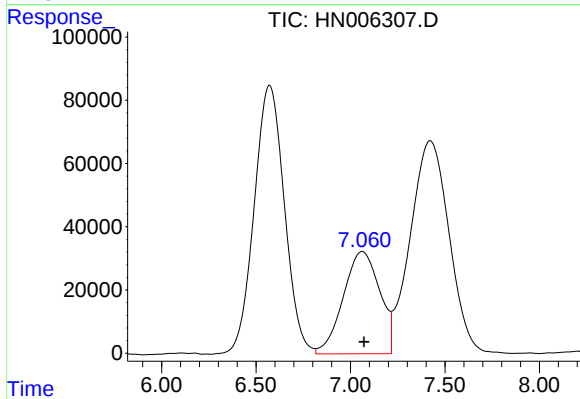

#10 2-Amino-4,6-dinitrotoluene

R.T.: 7.062 min
Delta R.T.: -0.009 min
Response: 4344971
Conc: 377.43 ug/L

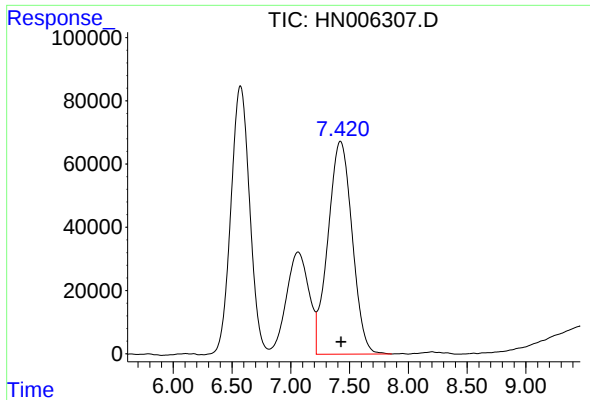

#11 4-Amino-2,6-dinitrotoluene

R.T.: 7.422 min
Delta R.T.: -0.007 min
Response: 9627332
Conc: 1572.47 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-GW03P-1014