

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN101514\HN006317.D\VWD1A.CH Vial: Instrument :
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN101514\HN006317.D\VWD1A.CH HPLC_N
 Acq On : 15-Oct-2014, 19:23 Operator: HNP ClientSampleId :
 Sample : F4244-01 Inst : G1314A YS09-GW04A-1014
 Misc : Multiplr: 1.00
 IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
 Quant Time: Oct 16 11:11 2014 Quant Results File: HN100214.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
 Title :
 Last Update : Fri Oct 03 10:34:01 2014
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.31	1136041	285.831 ug/L

Target Compounds

 Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.



HN006317.D HN100214.M Fri Oct 17 18:59:58 2014 RPT1


Quantitation Report

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN101514\HN006317.D\VWD1A.CH Vial: Instrument :
Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN101514\HN006317.D\VWD1A.CH HPLC_N
Acq On : 15-Oct-2014, 19:23 Operator: HNP ClientSampleId :
Sample : F4244-01 Inst : G1314A YS09-GW04A-1014
Misc : Multiplr: 1.00
IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
Quant Time: Oct 16 11:11 2014 Quant Results File: HN100214.RES

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Title :
Last Update : Fri Oct 03 10:34:01 2014
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

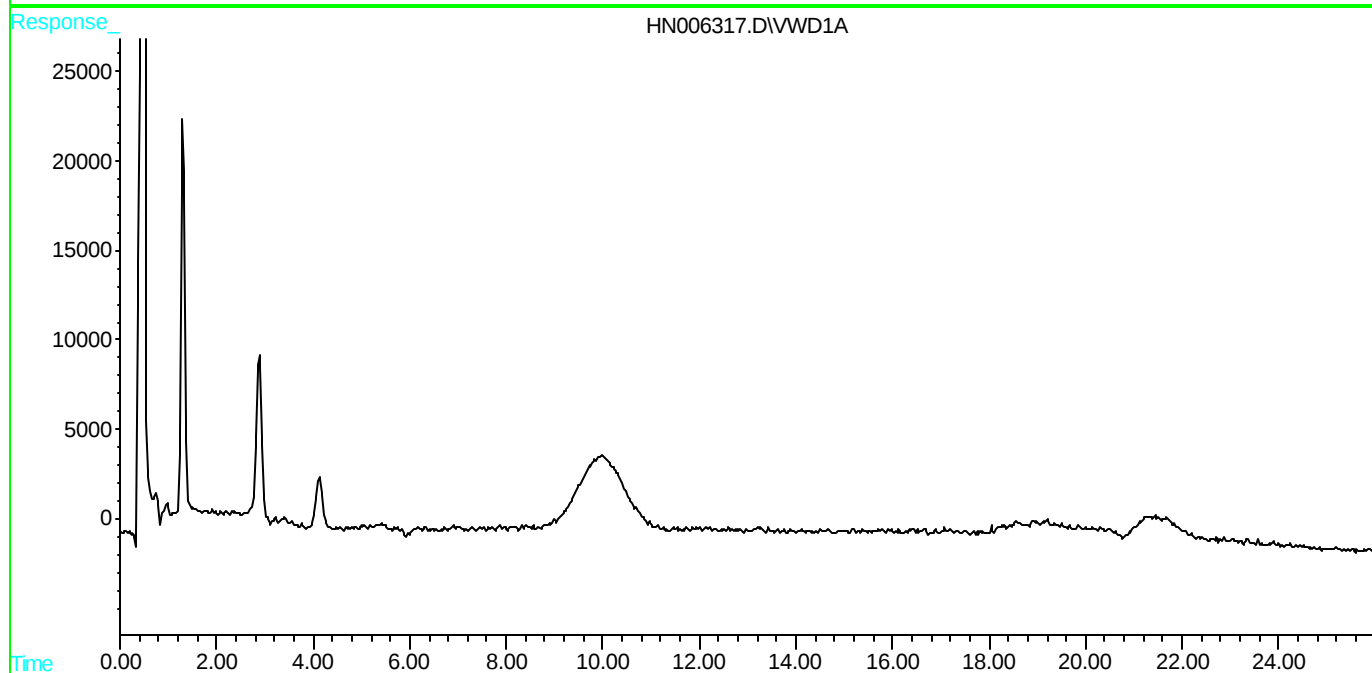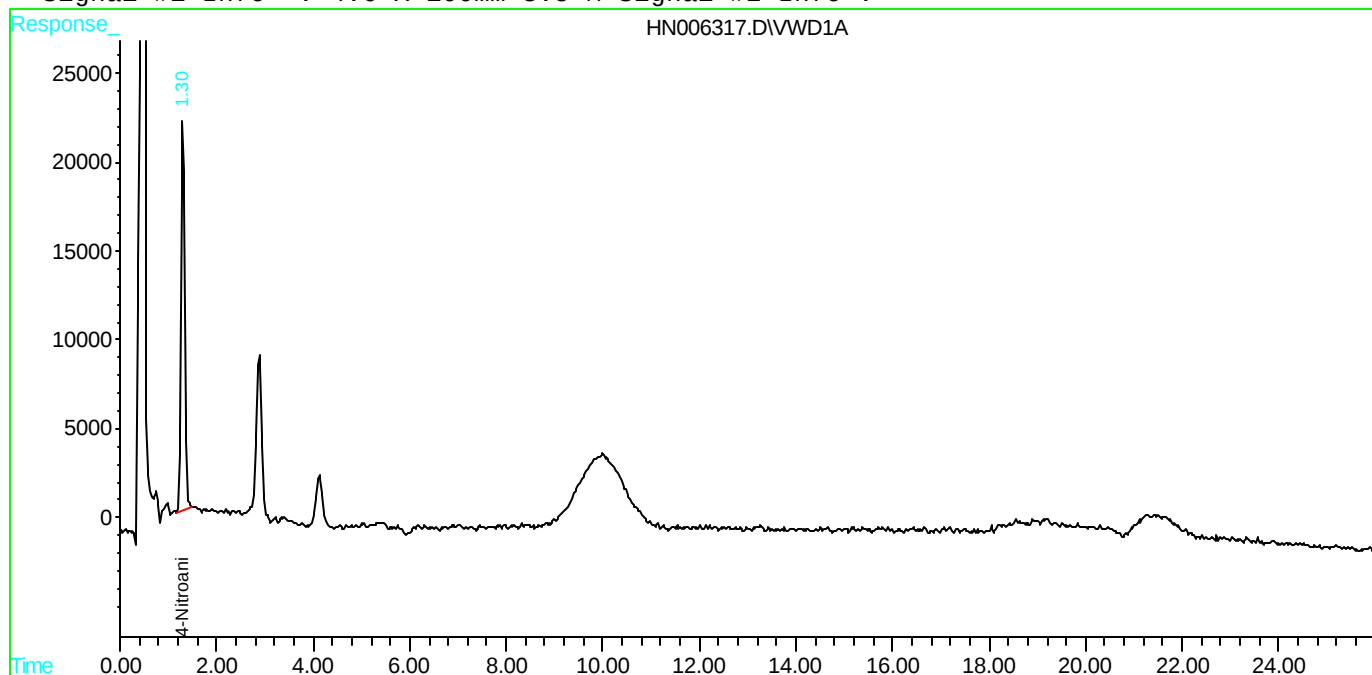

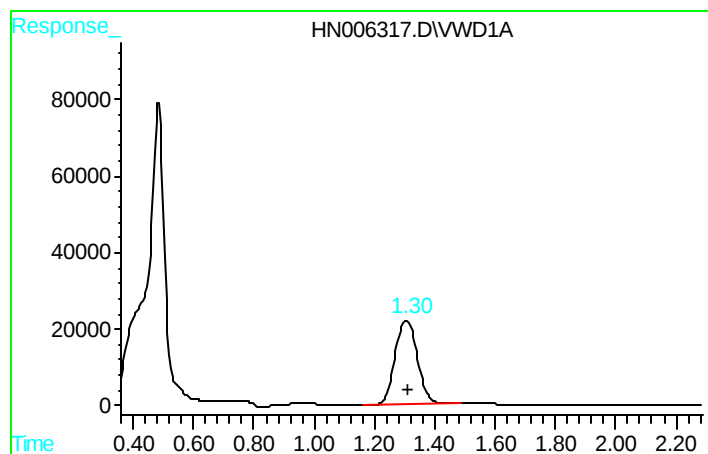

#1 4-Nitroaniline

R.T.: 1.306 min
Delta R.T.: -0.002 min
Response: 1136041
Conc: 285.83 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS09-GW04A-1014