

Signal #1 : X:\HPCHEM1\HPLC N\DATA\HN101514\HN006330.D\VWD1A.CH Vial: 29
Signal #2 : X:\HPCHEM1\HPLC N\DATA\HN101514\HN006330.D\VWD1A.CH
Acq On : 16-Oct-2014, 01:27 Operator: HNP
Sample : F4244-13 Inst : G1314A
Misc : Multiplr: 1.00
IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
Quant Time: Oct 16 11:37 2014 Quant Results File: HN100214.RES

Instrument :
HPLC_N
ClientSampleId :
YS19-GW13P-1014

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Title :
Last Update : Fri Oct 03 10:34:01 2014
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.31	1107386	278.621 ug/L

Target Compounds

Analyst Signature: _____ Analyst Name: _____ Date: _____

-----REASONS FOR MANUAL INTEGRATIONS-----

Poor resolution of peaks exhibited on chromatogram.Compound #:

Peak Integrated by software incorrectly.Compound #:

OTHER:

Compound #: _____

(f)=RT Delta > 1/2 Window

(m)=manual int.

HN006330.D HN100214.M

Thu Oct 30 05:15:38 2014



Quantitation Report


Signal #1 : X:\HPCHEM1\HPLC N\DATA\HN101514\HN006330.D\VWD1A.CH Vial: 29
 Signal #2 : X:\HPCHEM1\HPLC N\DATA\HN101514\HN006330.D\VWD1A.CH
 Acq On : 16-Oct-2014, 01:27 Operator: HNP
 Sample : F4244-13 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
 Quant Time: Oct 16 11:37 2014 Quant Results File: HN100214.RES

Instrument :
 HPLC_N
 ClientSampleId :
 YS19-GW13P-1014

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
 Title :
 Last Update : Fri Oct 03 10:34:01 2014
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

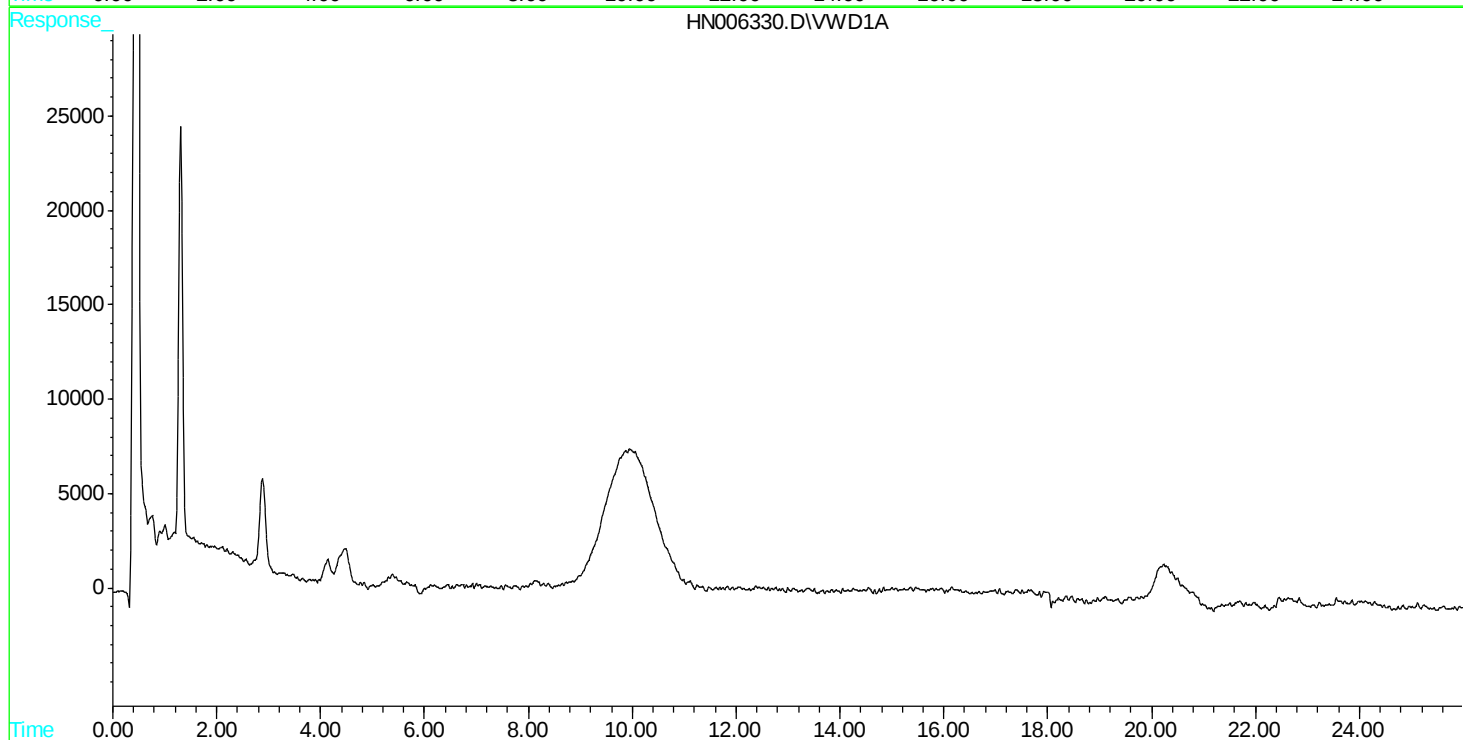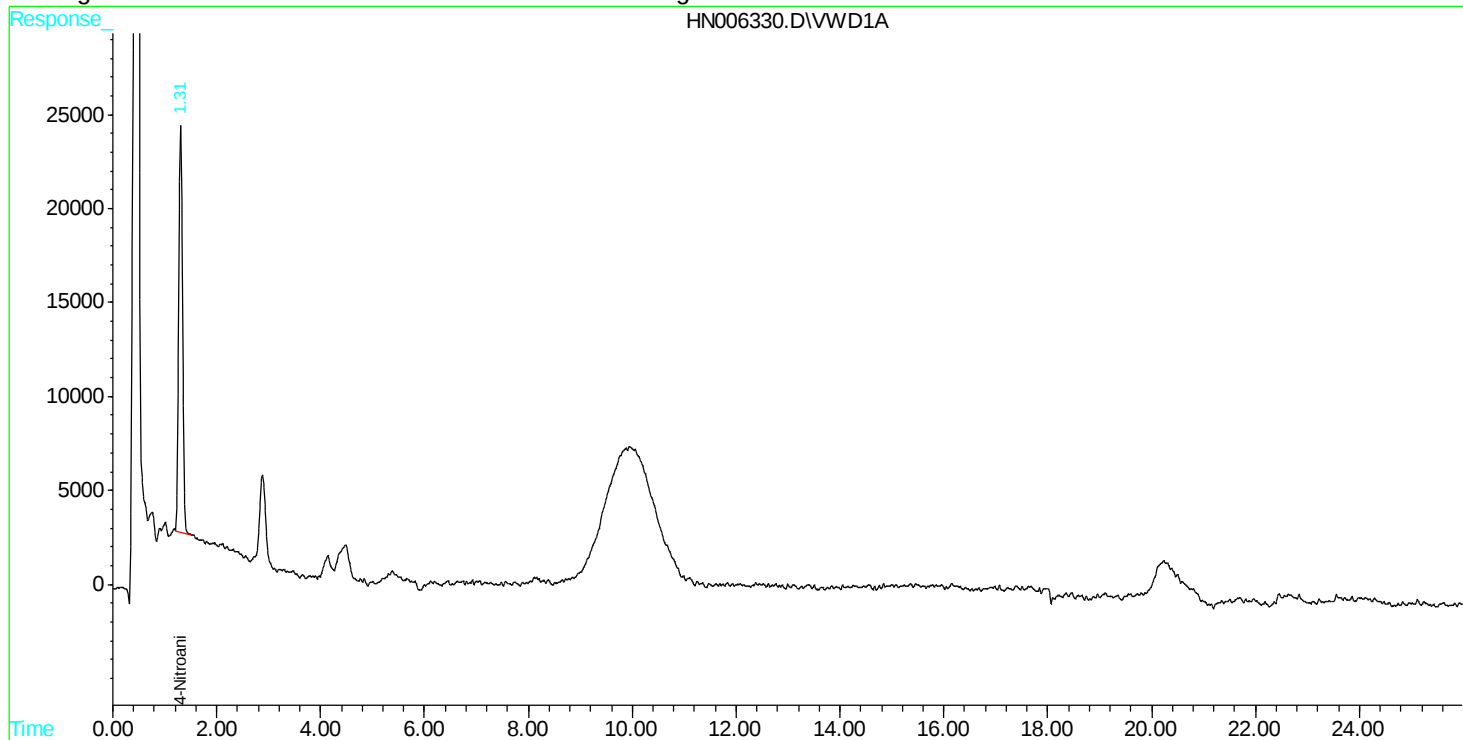

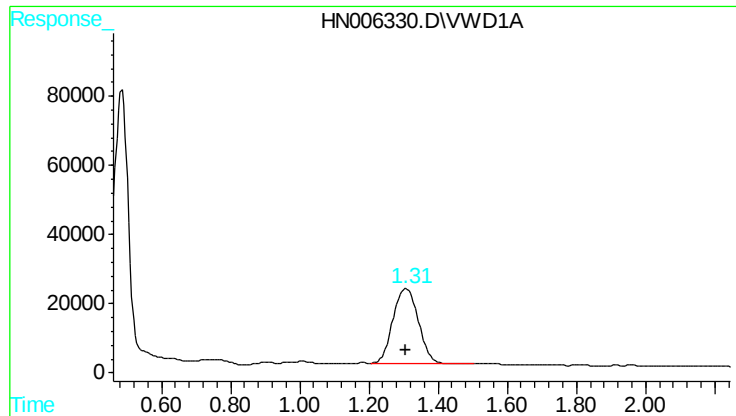

#1 4-Nitroaniline

R.T.: 1.308 min
Delta R.T.: 0.000 min
Response: 1107386
Conc: 278.62 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-GW13P-1014