

Data Path : Z:\HPCHEM1\HPLC\_N\Data\HN101714\  
Data File : HN006404.D  
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
Acq On : 17-Oct-2014, 13:43  
Operator : HNP  
Sample : HSTDCCC005  
Misc :  
ALS Vial : 51 Sample Multiplier: 1

Instrument :  
HPLC\_N  
ClientSampleId :  
HSTDCCC005

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 05 16:44:42 2015  
Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN1016NG.M  
Quant Title :  
QLast Update : Fri Oct 17 04:15:53 2014  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

| Compound                    | R.T.  | Response | Conc Units  |
|-----------------------------|-------|----------|-------------|
| -----                       |       |          |             |
| System Monitoring Compounds |       |          |             |
| 1) S 4-Nitroaniline         | 1.305 | 18596773 | 4.682 ng/ul |
|                             |       |          |             |
| Target Compounds            |       |          |             |
| 2) T Nitroglycerin          | 6.070 | 37411670 | 4.885 ng/ul |
| -----                       |       |          |             |

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC\_N\Data\HN101714\  
Data File : HN006404.D  
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
Acq On : 17-Oct-2014, 13:43  
Operator : HNP  
Sample : HSTDCCC005  
Misc :  
ALS Vial : 51 Sample Multiplier: 1

Instrument :  
HPLC\_N  
ClientSampleId :  
HSTDCCC005

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 05 16:44:42 2015  
Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN1016NG.M  
Quant Title :  
QLast Update : Fri Oct 17 04:15:53 2014  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

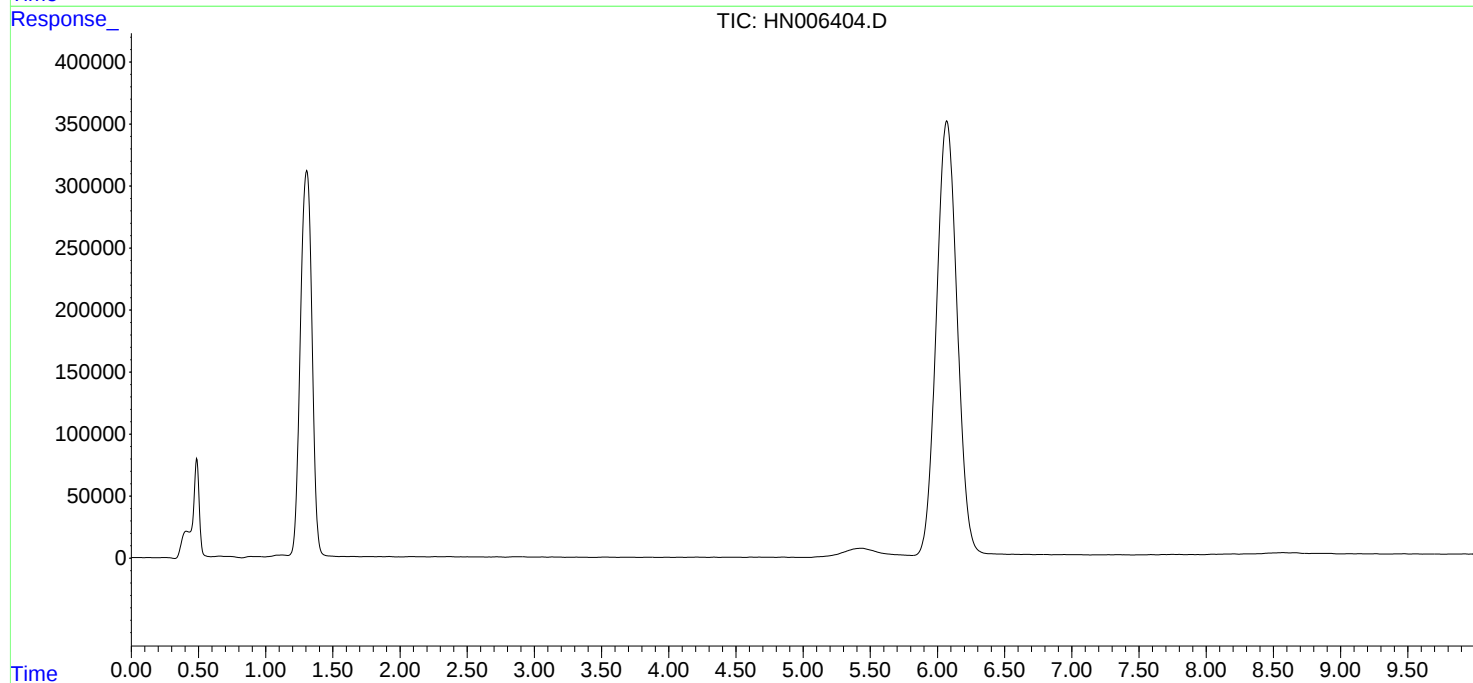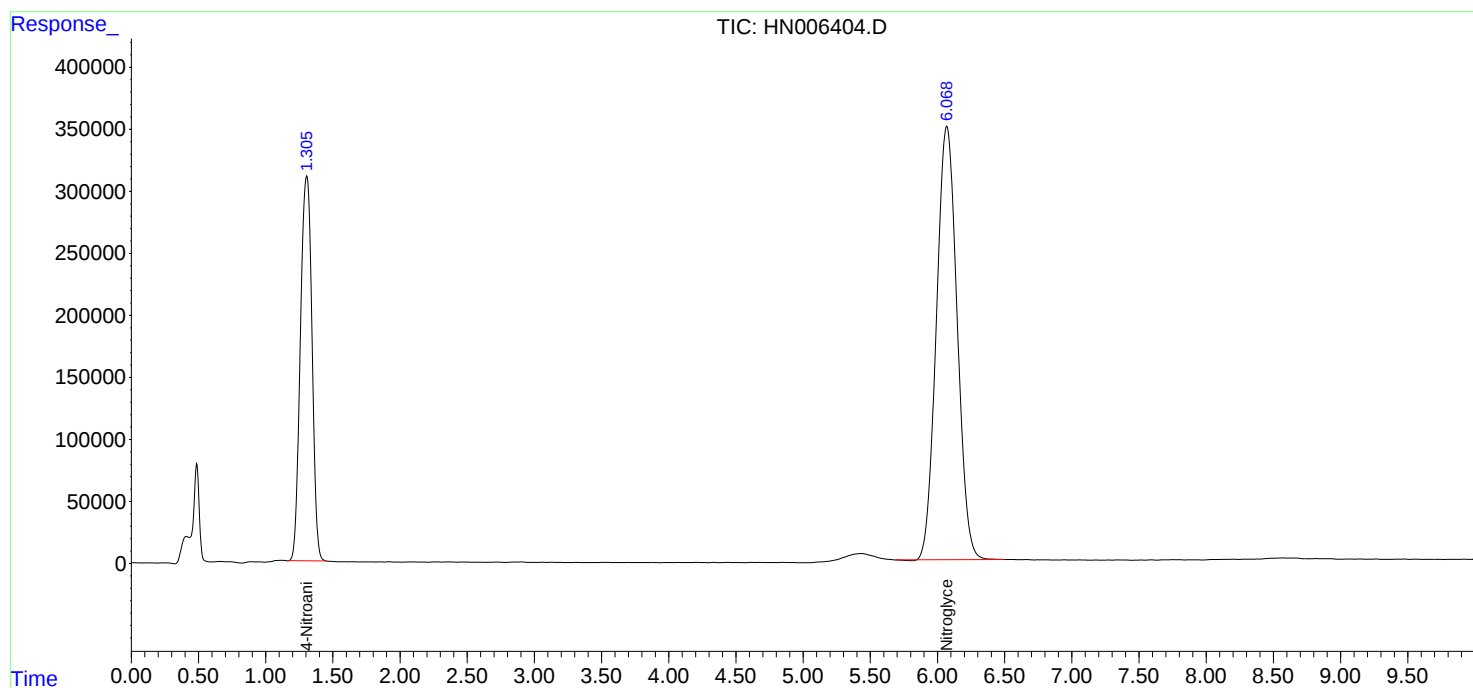


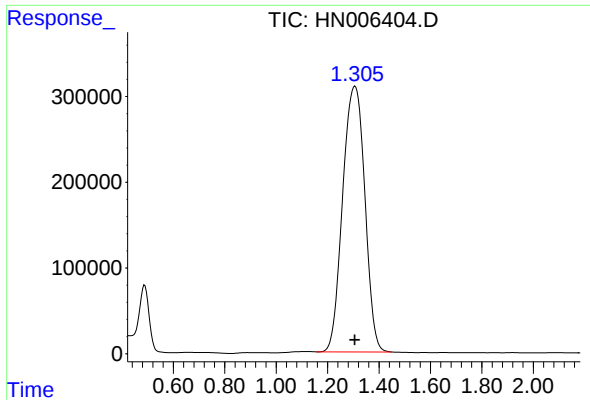

#1 4-Nitroaniline

R.T.: 1.305 min  
Delta R.T.: 0.000 min  
Response: 18596773  
Conc: 4.68 ng/ul

Instrument :  
HPLC\_N  
ClientSampleId :  
HSTDCCC005

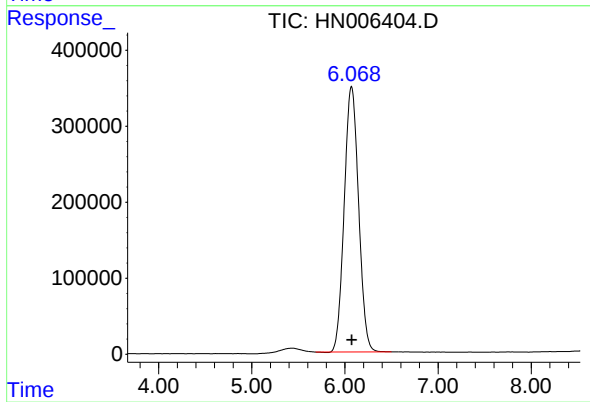

#2 Nitroglycerin

R.T.: 6.070 min  
Delta R.T.: -0.004 min  
Response: 37411670  
Conc: 4.88 ng/ul