

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN102314\
 Data File : HN006510.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 23-Oct-2014, 21:01
 Operator : HNP
 Sample : F4325-07
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 YS19-SS14-1014

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 02:06:23 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
 Quant Title :
 QLast Update : Mon Mar 09 14:56:25 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.305	631508	185.345 ug/L
Target Compounds			
4) T 1,3,5-Trinitrobenzene	2.671	369631	34.431 ug/L
9) T 2,4,6-Trinitrotoluene	6.582	2958150	269.682 ug/L
10) T 2-Amino-4,6-dinitroto...	7.089f	318834	27.695 ug/L
12) T 2,4-Dinitrotoluene	8.232f	246568	15.993 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN102314\
Data File : HN006510.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 23-Oct-2014, 21:01
Operator : HNP
Sample : F4325-07
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
YS19-SS14-1014

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 02:06:23 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Quant Title :
QLast Update : Mon Mar 09 14:56:25 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

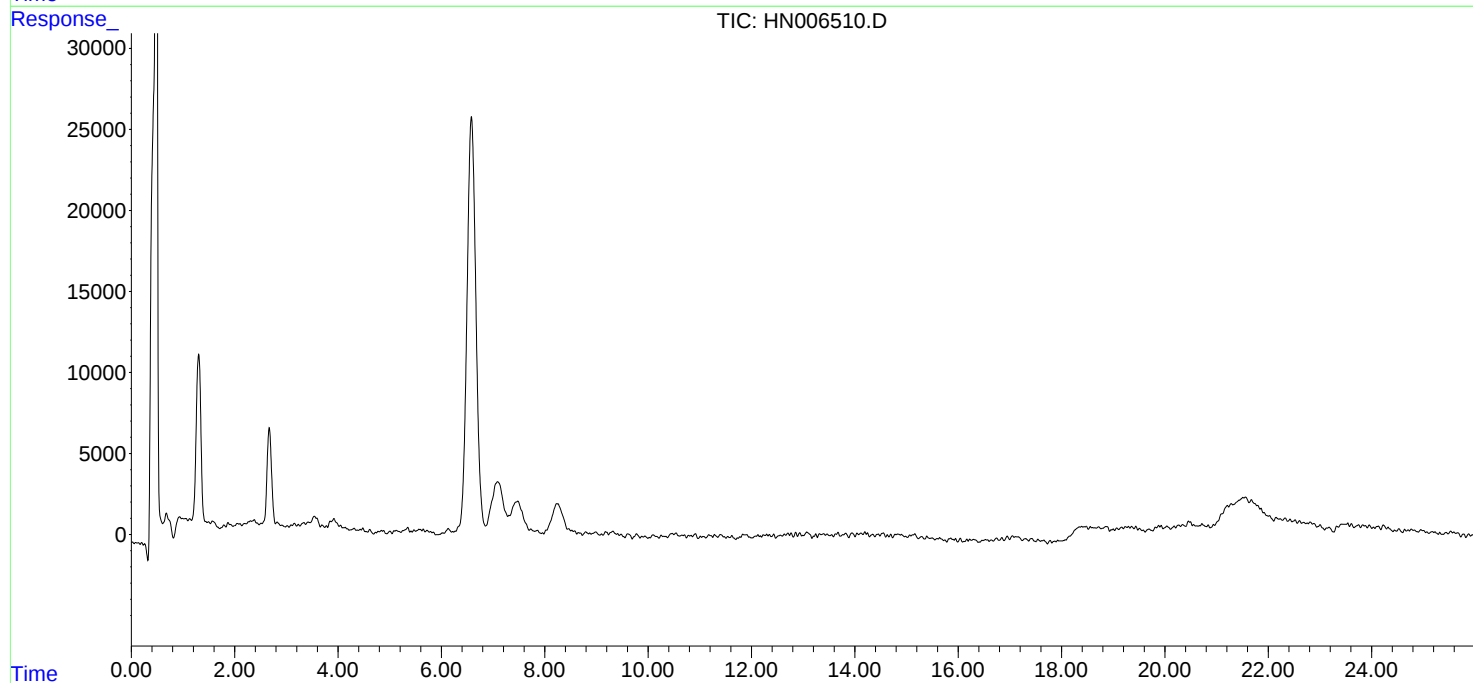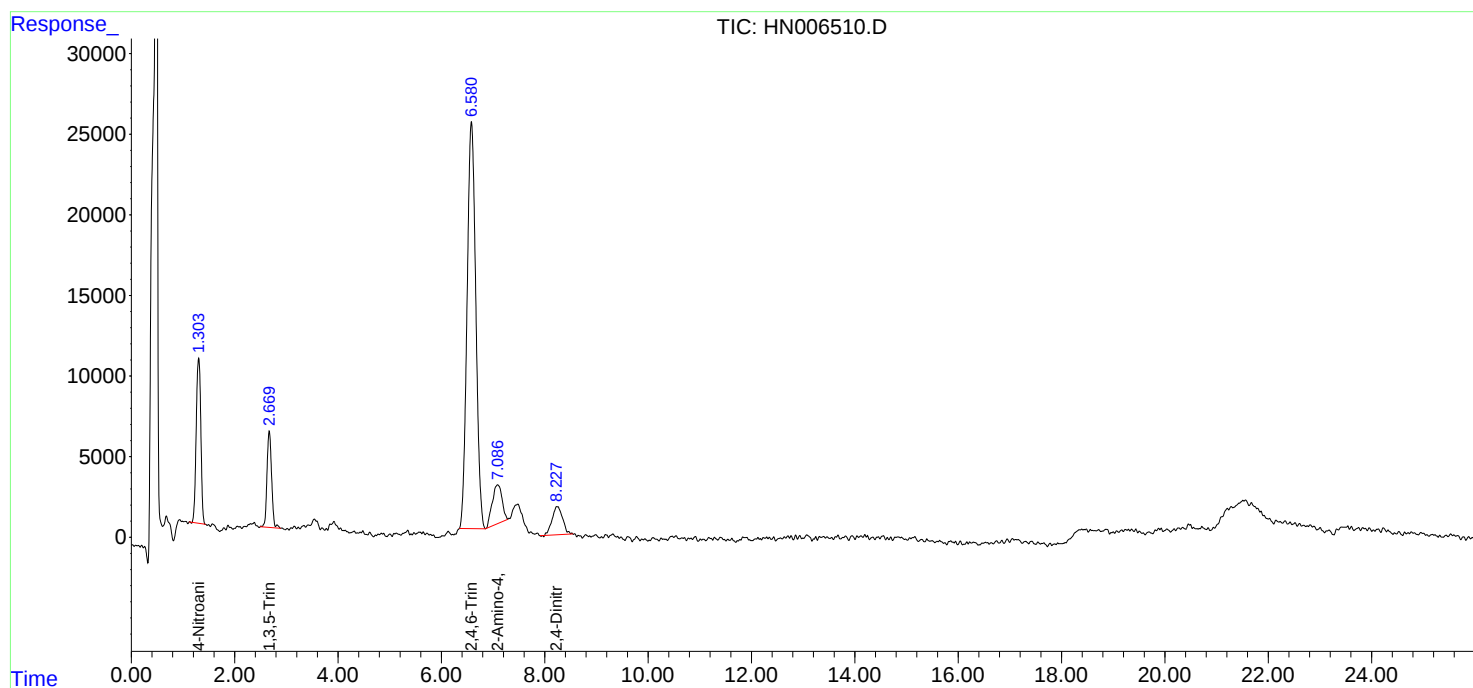


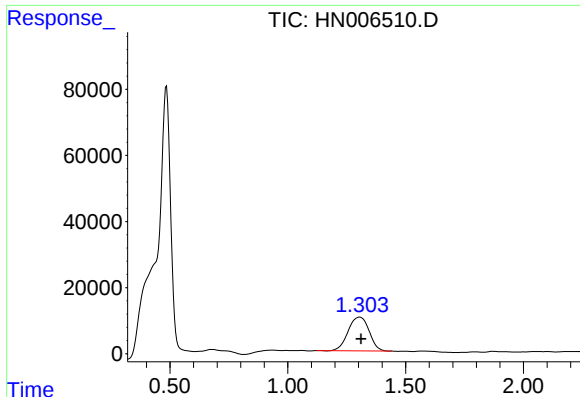

#1 4-Nitroaniline


R.T.: 1.305 min
Delta R.T.: -0.005 min
Response: 631508
Conc: 185.35 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-SS14-1014

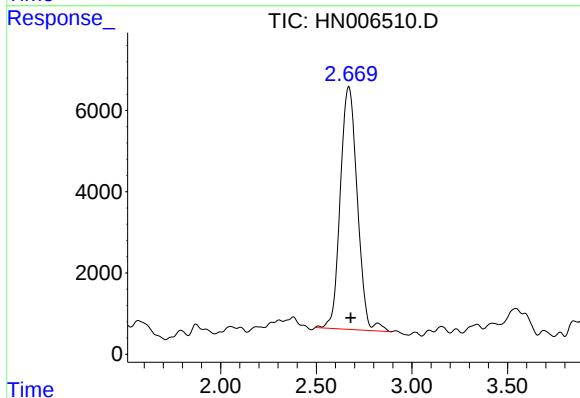


#4 1,3,5-Trinitrobenzene

R.T.: 2.671 min
Delta R.T.: -0.010 min
Response: 369631
Conc: 34.43 ug/L

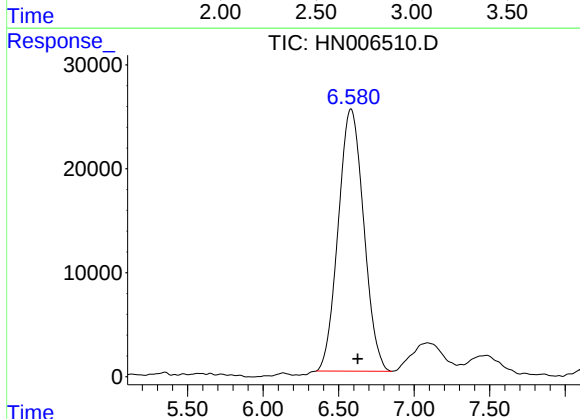


#9 2,4,6-Trinitrotoluene

R.T.: 6.582 min
Delta R.T.: -0.045 min
Response: 2958150
Conc: 269.68 ug/L

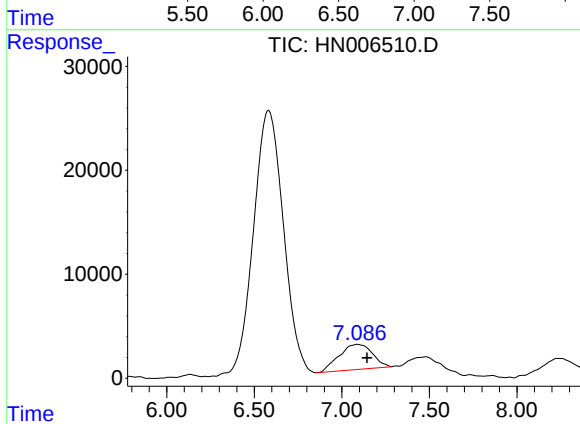

#10 2-Amino-4,6-dinitrotoluene

R.T.: 7.089 min
Delta R.T.: -0.055 min
Response: 318834
Conc: 27.70 ug/L

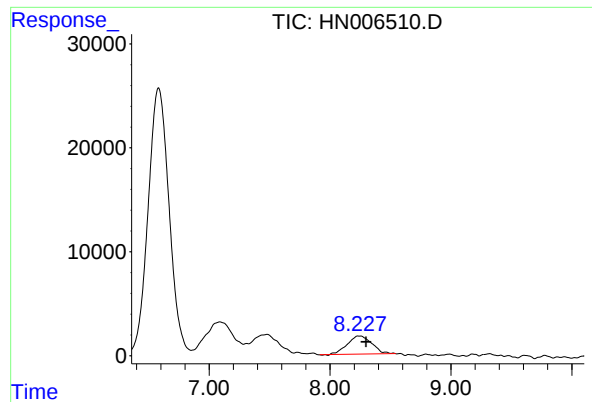

#12 2,4-Dinitrotoluene

R.T.: 8.232 min
Delta R.T.: -0.067 min
Response: 246568
Conc: 15.99 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-SS14-1014