

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN102314\
 Data File : HN006511.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 23-Oct-2014, 21:29
 Operator : HNP
 Sample : F4325-08
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 YS19-SB14-1014

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 02:06:34 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
 Quant Title :
 QLast Update : Mon Mar 09 14:56:25 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.303	635298	186.458 ug/L
Target Compounds			
4) T 1,3,5-Trinitrobenzene	2.667	12849244	1196.890 ug/L
6) T 3,5-Dinitroaniline	3.921	834158	71.744 ug/L
9) T 2,4,6-Trinitrotoluene	6.582	16061629	1464.269 ug/L
10) T 2-Amino-4,6-dinitroto...	7.081f	1813689	157.546 ug/L
11) T 4-Amino-2,6-dinitroto...	7.476	1016658	166.055 ug/L
12) T 2,4-Dinitrotoluene	8.246f	974256	63.192 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN102314\
Data File : HN006511.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 23-Oct-2014, 21:29
Operator : HNP
Sample : F4325-08
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
YS19-SB14-1014

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 02:06:34 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Quant Title :
QLast Update : Mon Mar 09 14:56:25 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

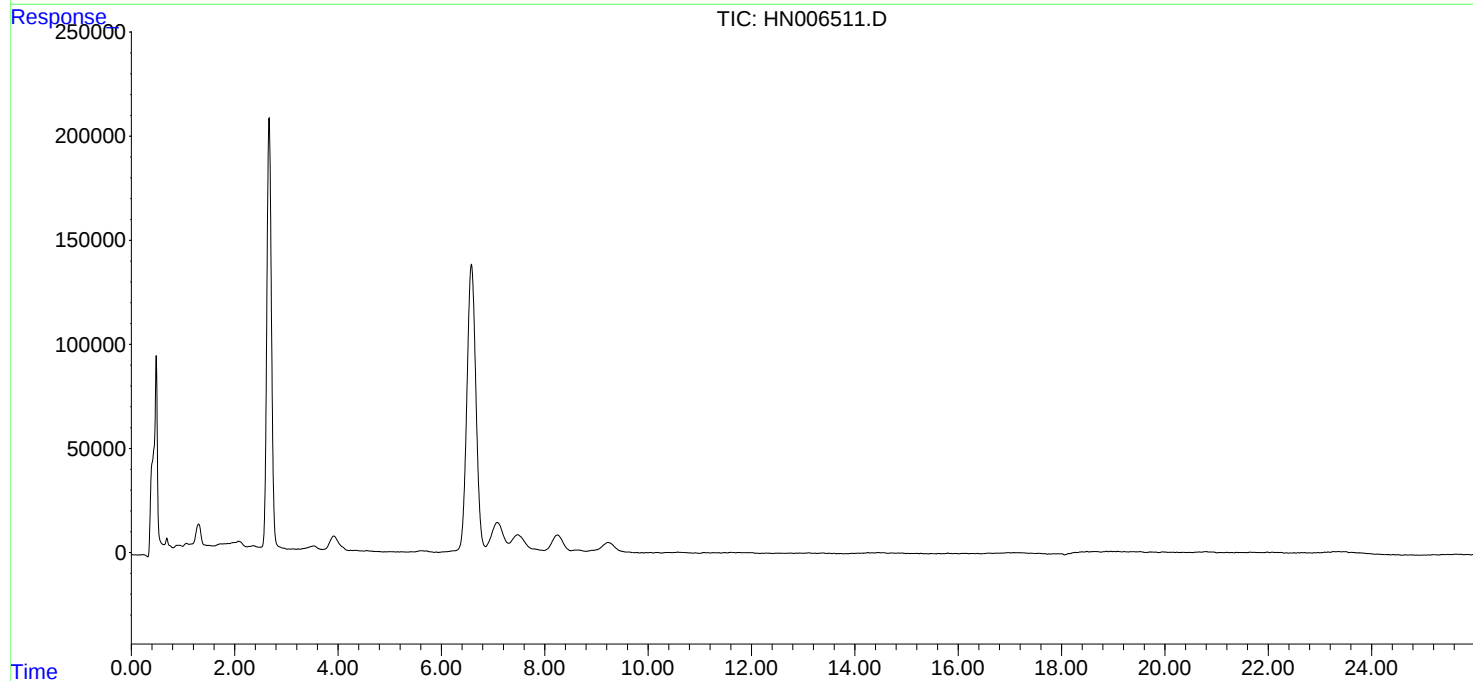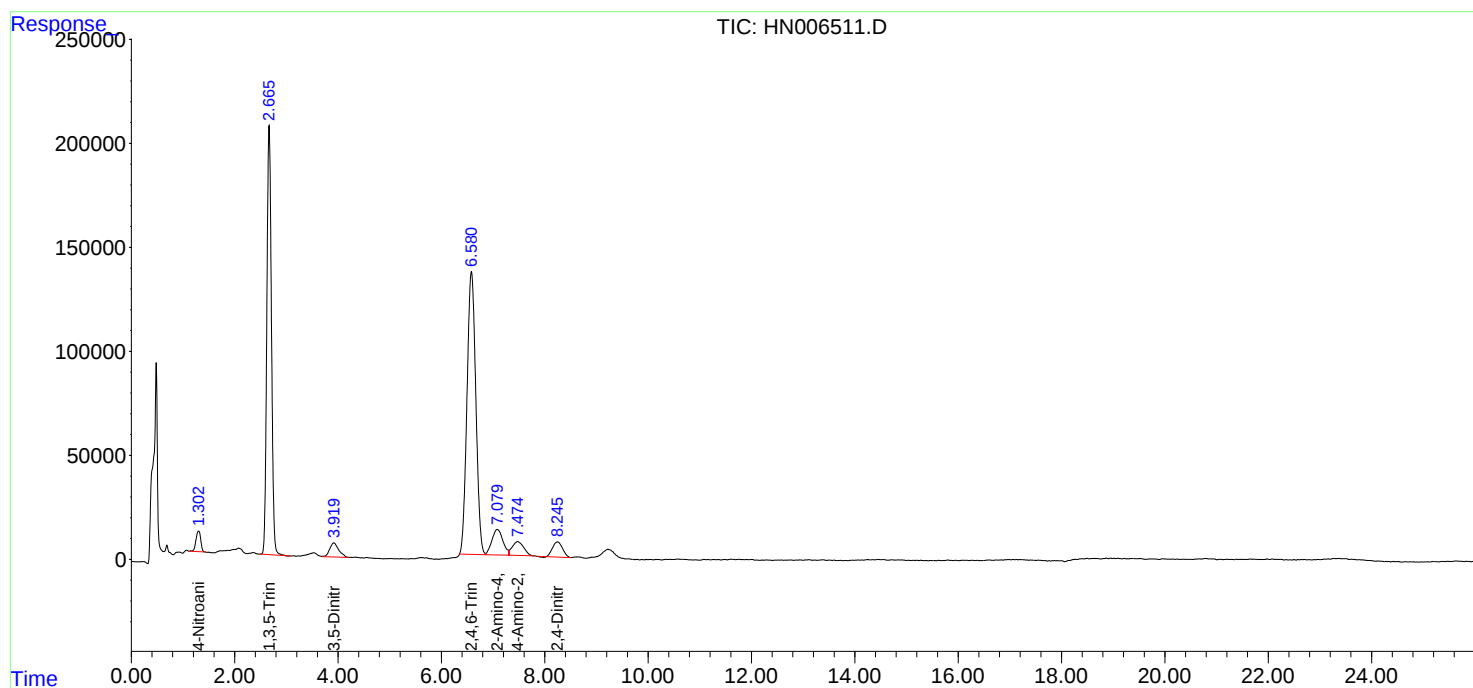


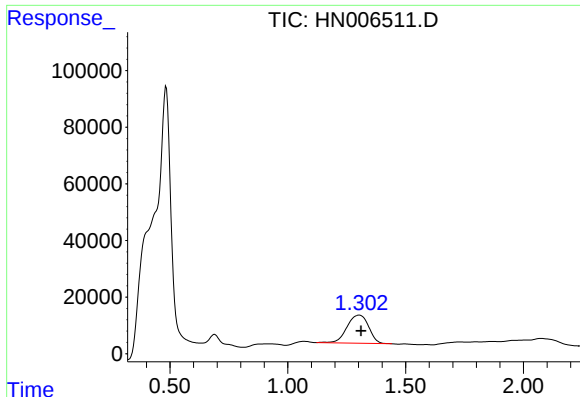

#1 4-Nitroaniline


R.T.: 1.303 min
Delta R.T.: -0.007 min
Response: 635298
Conc: 186.46 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-SB14-1014

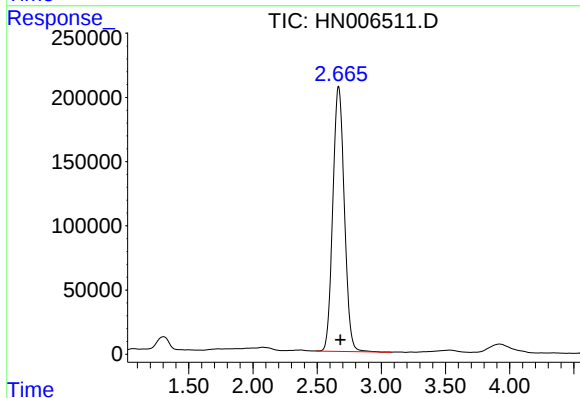


#4 1,3,5-Trinitrobenzene

R.T.: 2.667 min
Delta R.T.: -0.013 min
Response: 12849244
Conc: 1196.89 ug/L

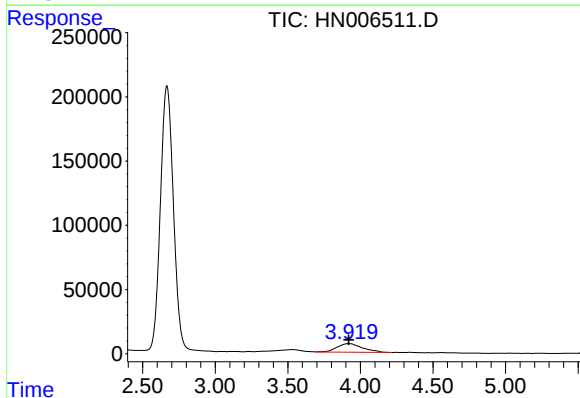


#6 3,5-Dinitroaniline

R.T.: 3.921 min
Delta R.T.: 0.000 min
Response: 834158
Conc: 71.74 ug/L

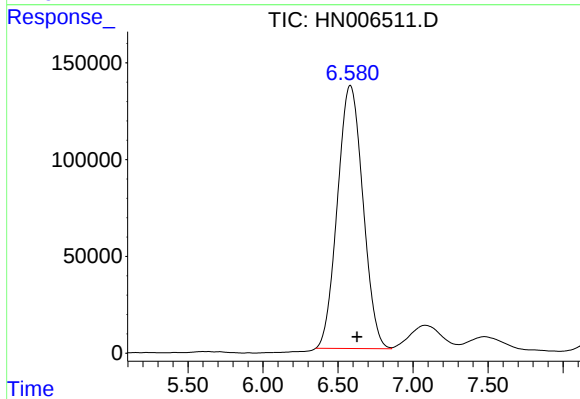

#9 2,4,6-Trinitrotoluene


R.T.: 6.582 min
Delta R.T.: -0.045 min
Response: 16061629
Conc: 1464.27 ug/L

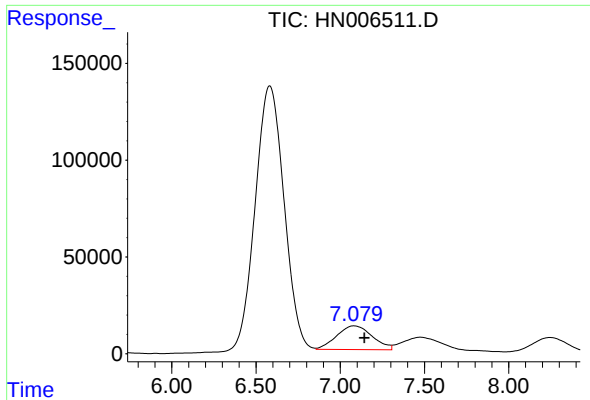

#10 2-Amino-4,6-dinitrotoluene


R.T.: 7.081 min
Delta R.T.: -0.063 min
Response: 1813689
Conc: 157.55 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-SB14-1014

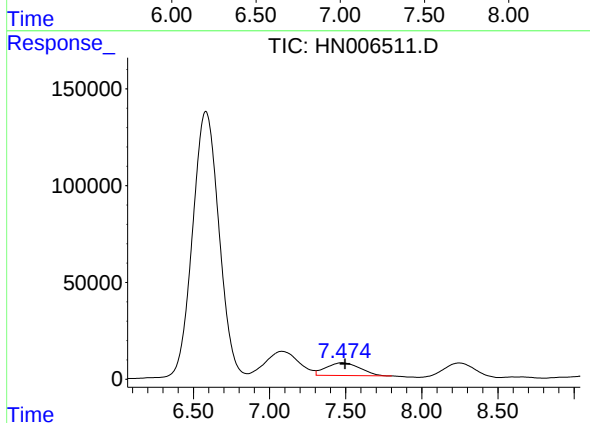

#11 4-Amino-2,6-dinitrotoluene

R.T.: 7.476 min
Delta R.T.: -0.020 min
Response: 1016658
Conc: 166.05 ug/L

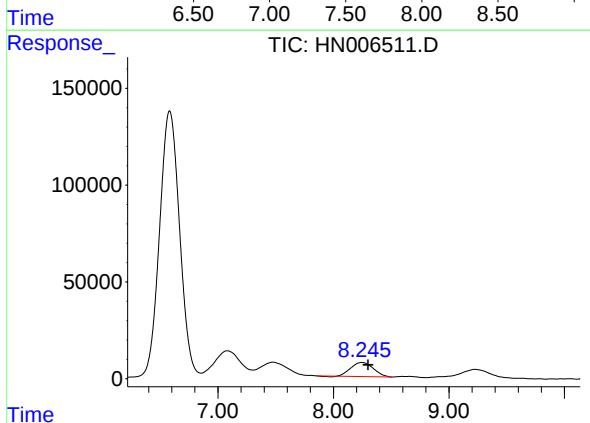

#12 2,4-Dinitrotoluene

R.T.: 8.246 min
Delta R.T.: -0.053 min
Response: 974256
Conc: 63.19 ug/L