

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN102314\
 Data File : HN006542.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 24-Oct-2014, 11:57
 Operator : HNP
 Sample : HSTDCCC0500
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDCCC0500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 02:16:52 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
 Quant Title :
 QLast Update : Mon Mar 09 14:56:25 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.309	1582659	464.505 ug/L
Target Compounds			
2) T HMX	0.873	2010147	445.909 ug/L
3) T RDX	1.696	2695760	514.172 ug/L
4) T 1,3,5-Trinitrobenzene	2.668	5527396	514.869 ug/L
5) T 1,3-Dinitrobenzene	3.539	8340470	511.227 ng/ml
6) T 3,5-Dinitroaniline	3.896	6020813	517.838 ug/L
7) T Nitrobenzene	4.778	5106403	507.055 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN102314\
Data File : HN006542.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 24-Oct-2014, 11:57
Operator : HNP
Sample : HSTDCCC0500
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 02:16:52 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Quant Title :
QLast Update : Mon Mar 09 14:56:25 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

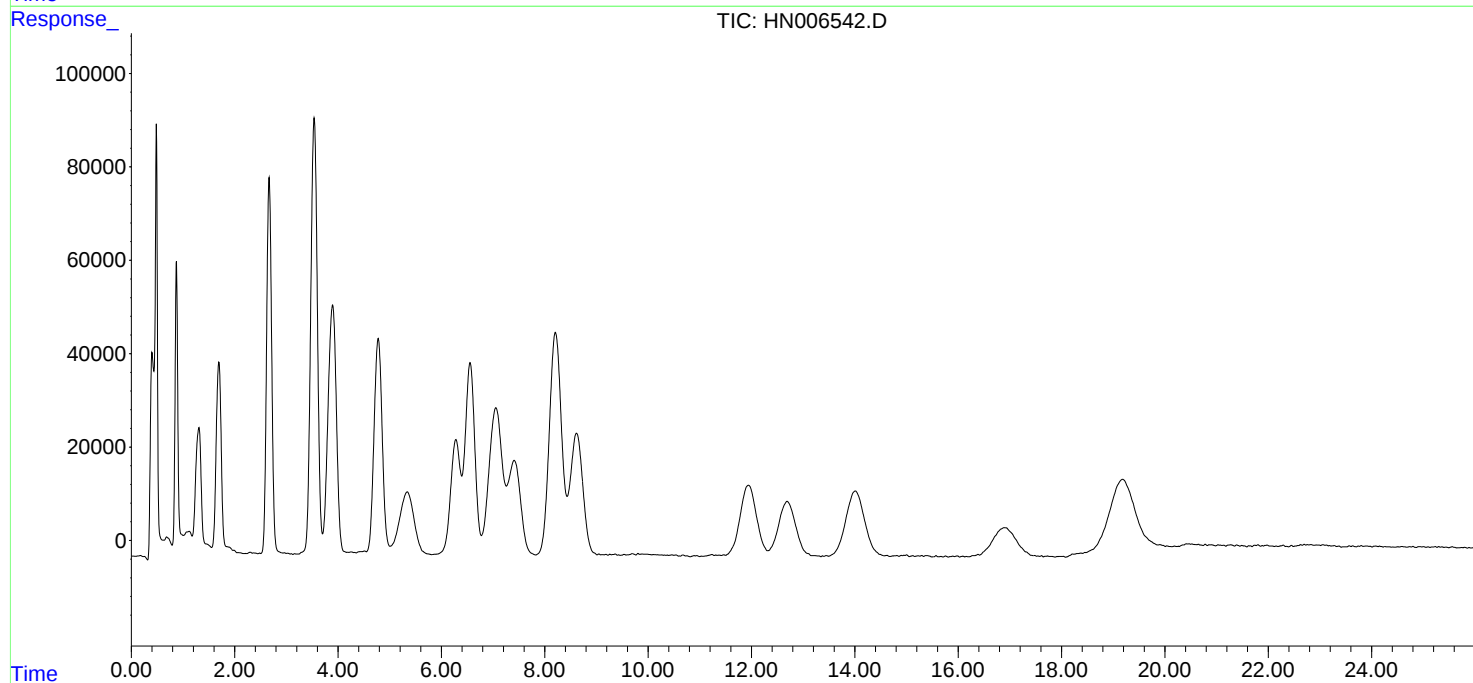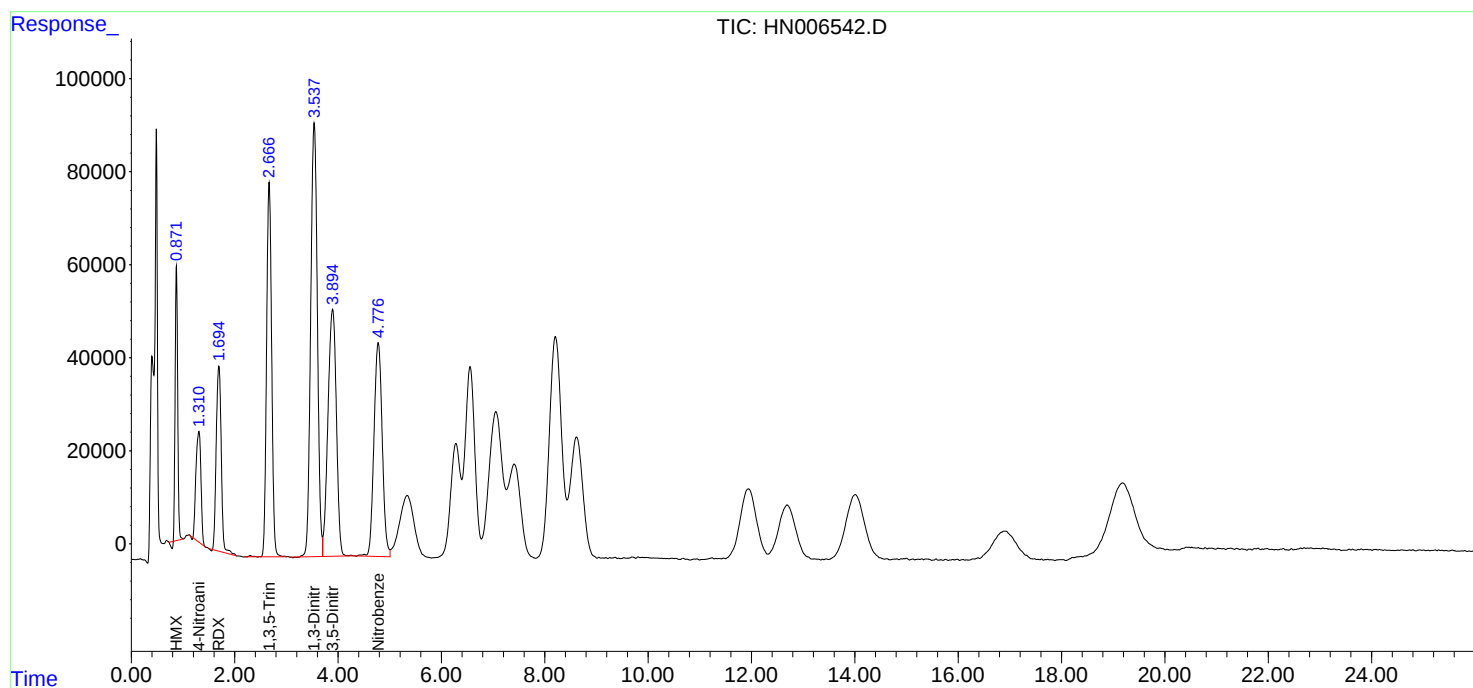


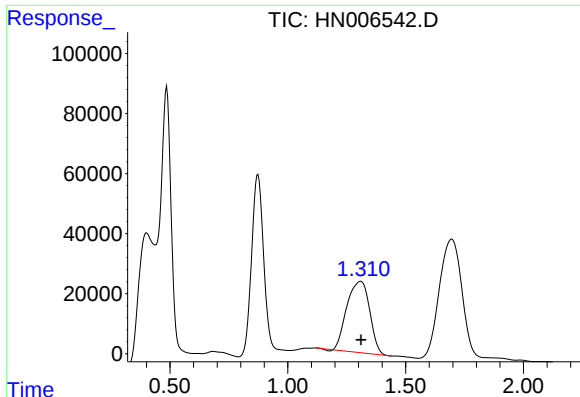

#1 4-Nitroaniline


R.T.: 1.309 min
Delta R.T.: -0.001 min
Response: 1582659
Conc: 464.50 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

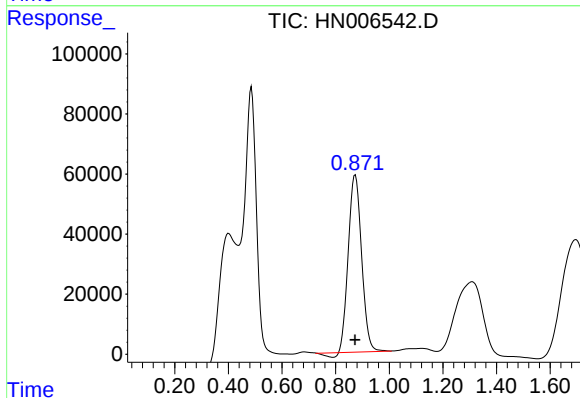


#2 HMX

R.T.: 0.873 min
Delta R.T.: 0.000 min
Response: 2010147
Conc: 445.91 ug/L

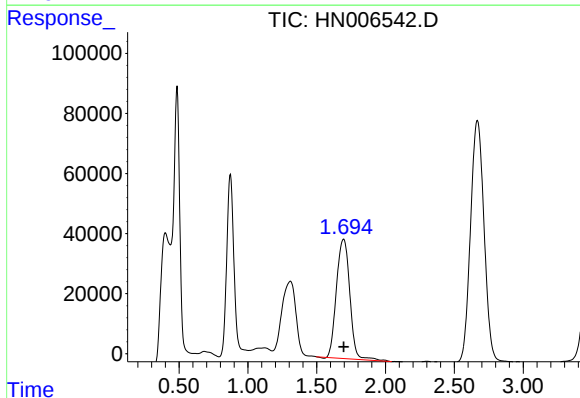


#3 RDX

R.T.: 1.696 min
Delta R.T.: -0.001 min
Response: 2695760
Conc: 514.17 ug/L

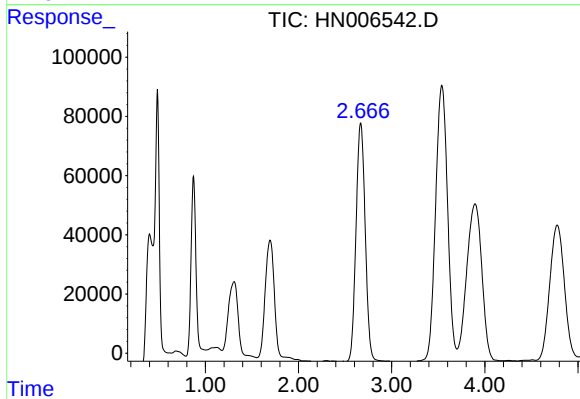

#4 1,3,5-Trinitrobenzene


R.T.: 2.668 min
Delta R.T.: -0.013 min
Response: 5527396
Conc: 514.87 ug/L

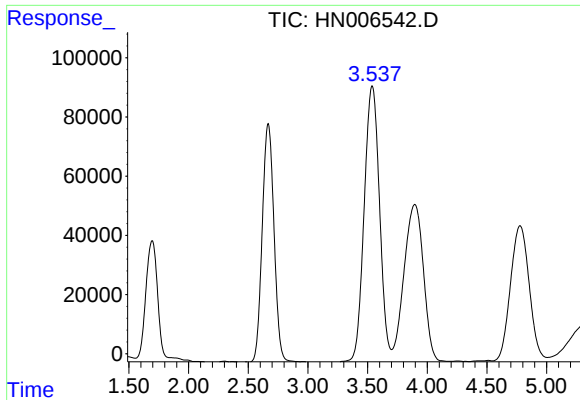

#5 1,3-Dinitrobenzene


R.T.: 3.539 min
Delta R.T.: -0.018 min
Response: 8340470
Conc: 511.23 ng/ml

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

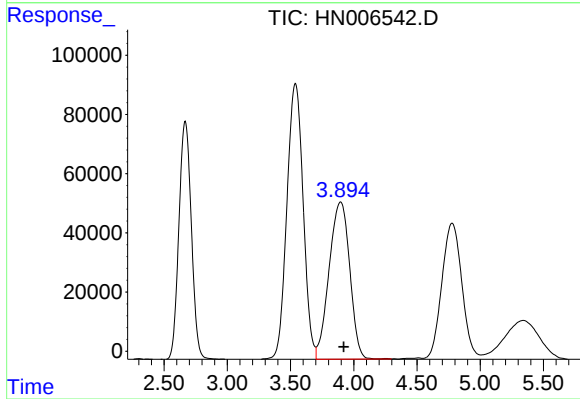

#6 3,5-Dinitroaniline

R.T.: 3.896 min
Delta R.T.: -0.024 min
Response: 6020813
Conc: 517.84 ug/L

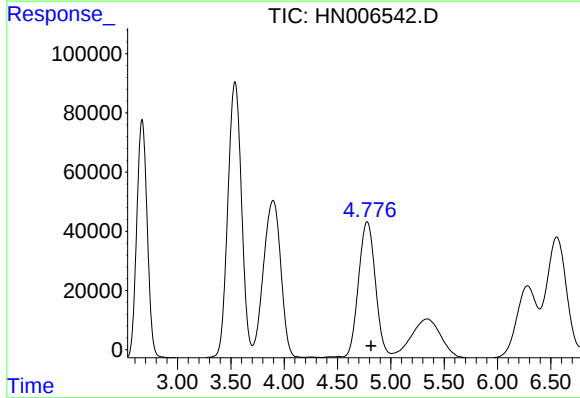

#7 Nitrobenzene

R.T.: 4.778 min
Delta R.T.: -0.036 min
Response: 5106403
Conc: 507.05 ug/L