

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN102314\
 Data File : HN006546.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 24-Oct-2014, 13:50
 Operator : HNP
 Sample : F4368-12MS
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 YS19-SS39-1014MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 02:17:38 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
 Quant Title :
 QLast Update : Mon Mar 09 14:56:25 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.302	568702	166.912 ug/L
Target Compounds			
2) T HMX	0.874	528847	117.314 ug/L
3) T RDX	1.694	635238	121.161 ug/L
4) T 1,3,5-Trinitrobenzene	2.666	1334531	124.310 ug/L
5) T 1,3-Dinitrobenzene	3.535	2145037	131.479 ng/ml
6) T 3,5-Dinitroaniline	3.887	1611498	138.602 ug/L
7) T Nitrobenzene	4.776	1337342	132.795 ug/L
9) T 2,4,6-Trinitrotoluene	6.564f	930957	84.871 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN102314\
Data File : HN006546.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 24-Oct-2014, 13:50
Operator : HNP
Sample : F4368-12MS
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
YS19-SS39-1014MS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 02:17:38 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Quant Title :
QLast Update : Mon Mar 09 14:56:25 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

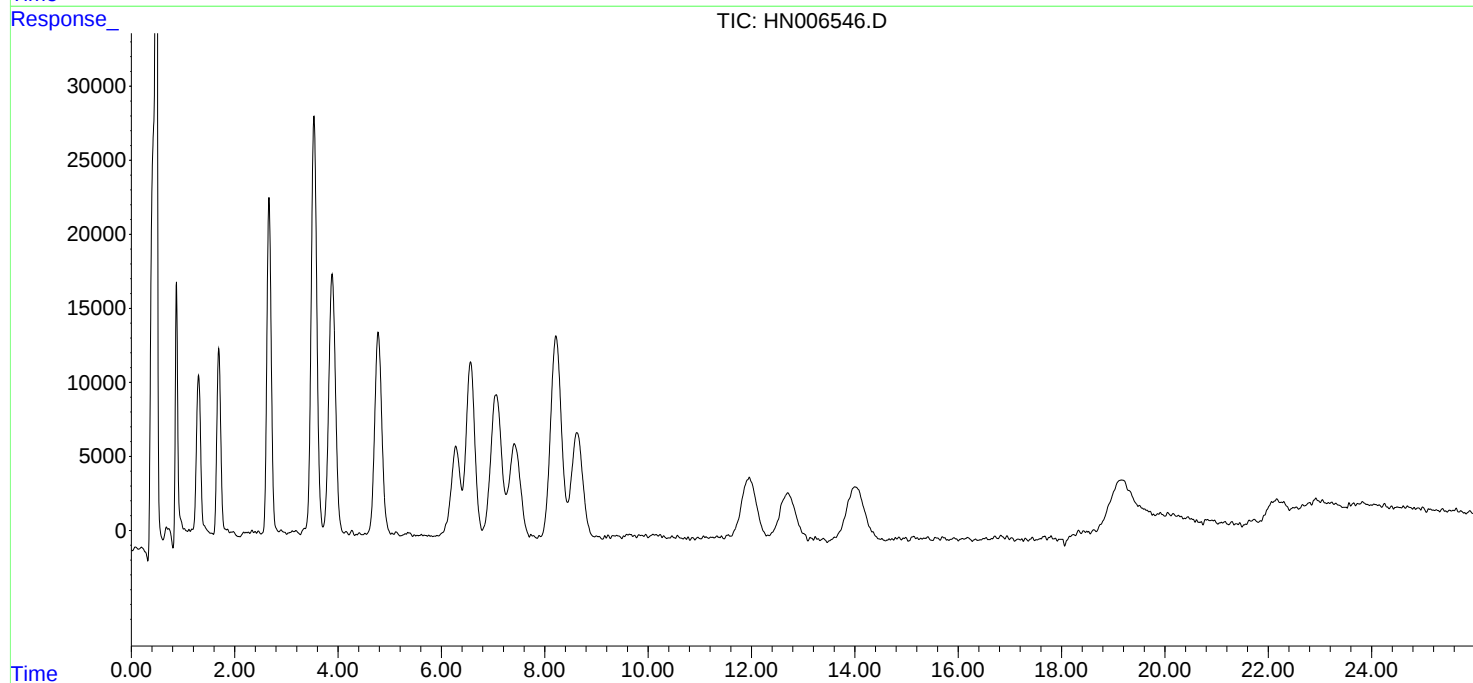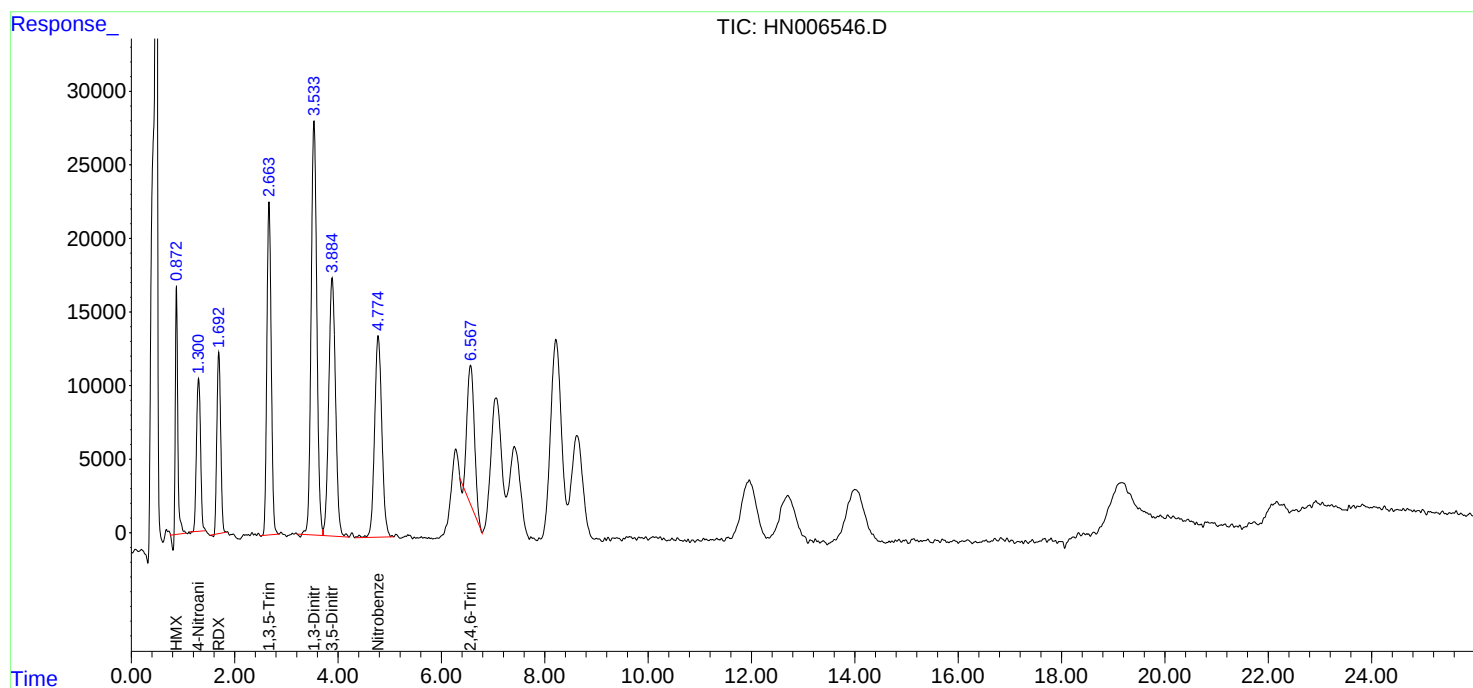


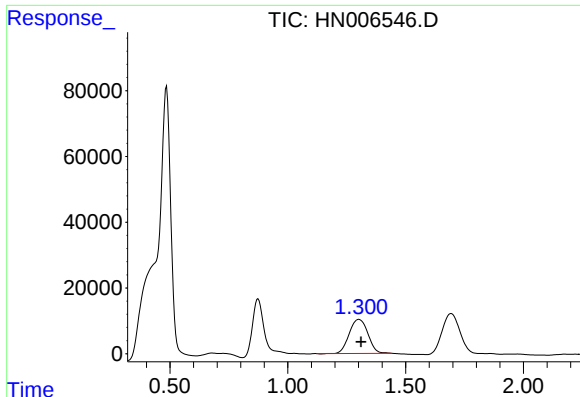

#1 4-Nitroaniline


R.T.: 1.302 min
Delta R.T.: -0.008 min
Response: 568702
Conc: 166.91 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-SS39-1014MS

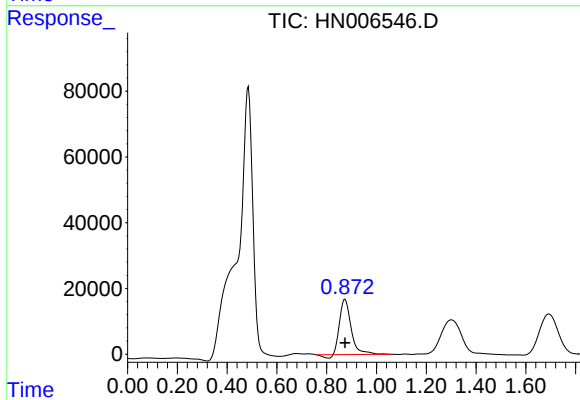


#2 HMX

R.T.: 0.874 min
Delta R.T.: 0.001 min
Response: 528847
Conc: 117.31 ug/L

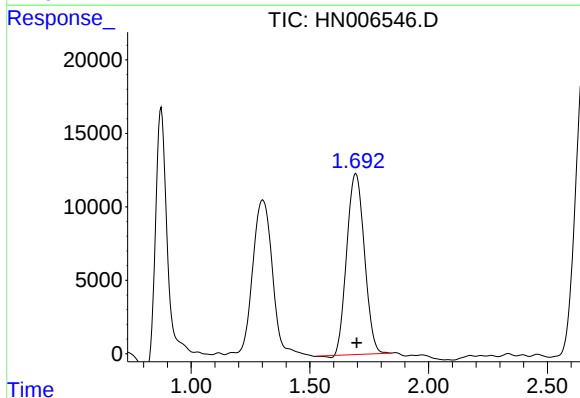


#3 RDX

R.T.: 1.694 min
Delta R.T.: -0.003 min
Response: 635238
Conc: 121.16 ug/L

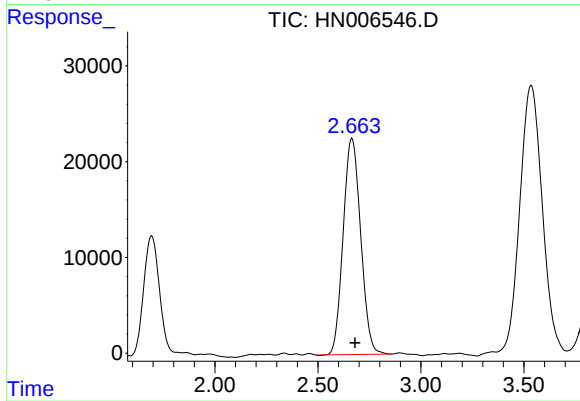

#4 1,3,5-Trinitrobenzene


R.T.: 2.666 min
Delta R.T.: -0.015 min
Response: 1334531
Conc: 124.31 ug/L

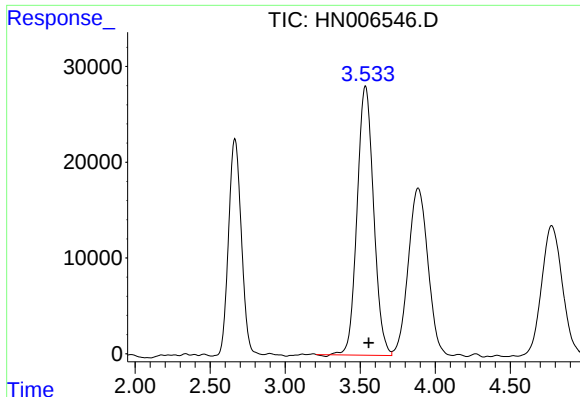

#5 1,3-Dinitrobenzene


R.T.: 3.535 min
Delta R.T.: -0.022 min
Response: 2145037
Conc: 131.48 ng/ml

Instrument :
HPLC_N
ClientSampleId :
YS19-SS39-1014MS

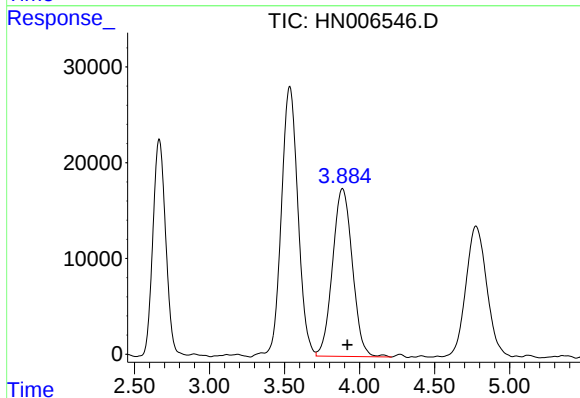


#6 3,5-Dinitroaniline

R.T.: 3.887 min
Delta R.T.: -0.034 min
Response: 1611498
Conc: 138.60 ug/L

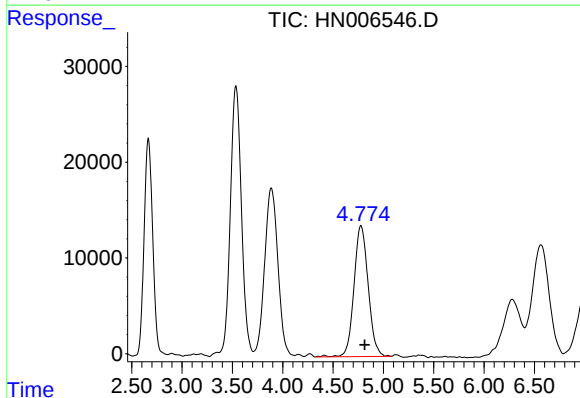

#7 Nitrobenzene

R.T.: 4.776 min
Delta R.T.: -0.037 min
Response: 1337342
Conc: 132.80 ug/L

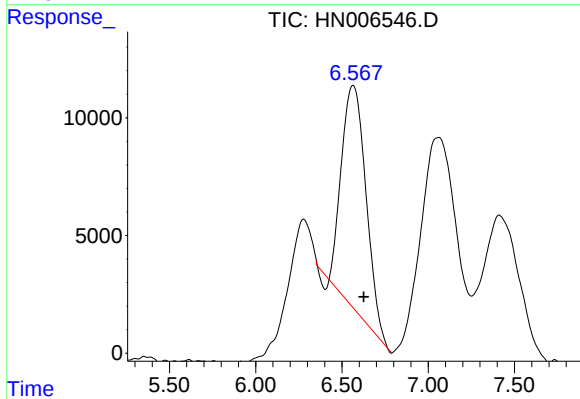

#9 2,4,6-Trinitrotoluene

R.T.: 6.564 min
Delta R.T.: -0.062 min
Response: 930957
Conc: 84.87 ug/L