

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN102314\
 Data File : HN006559.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 24-Oct-2014, 19:54
 Operator : HNP
 Sample : PB79759BS
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 PB79759BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 02:19:42 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
 Quant Title :
 QLast Update : Mon Mar 09 14:56:25 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.300	612796	179.853 ug/L
Target Compounds			
2) T HMX	0.870	532194	118.056 ug/L
3) T RDX	1.690	653695	124.682 ug/L
4) T 1,3,5-Trinitrobenzene	2.662	1340625	124.877 ug/L
5) T 1,3-Dinitrobenzene	3.534	2138510	131.079 ng/ml
6) T 3,5-Dinitroaniline	3.891	1621322	139.447 ug/L
7) T Nitrobenzene	4.779	1329118	131.979 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN102314\
Data File : HN006559.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 24-Oct-2014, 19:54
Operator : HNP
Sample : PB79759BS
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
PB79759BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 02:19:42 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Quant Title :
QLast Update : Mon Mar 09 14:56:25 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

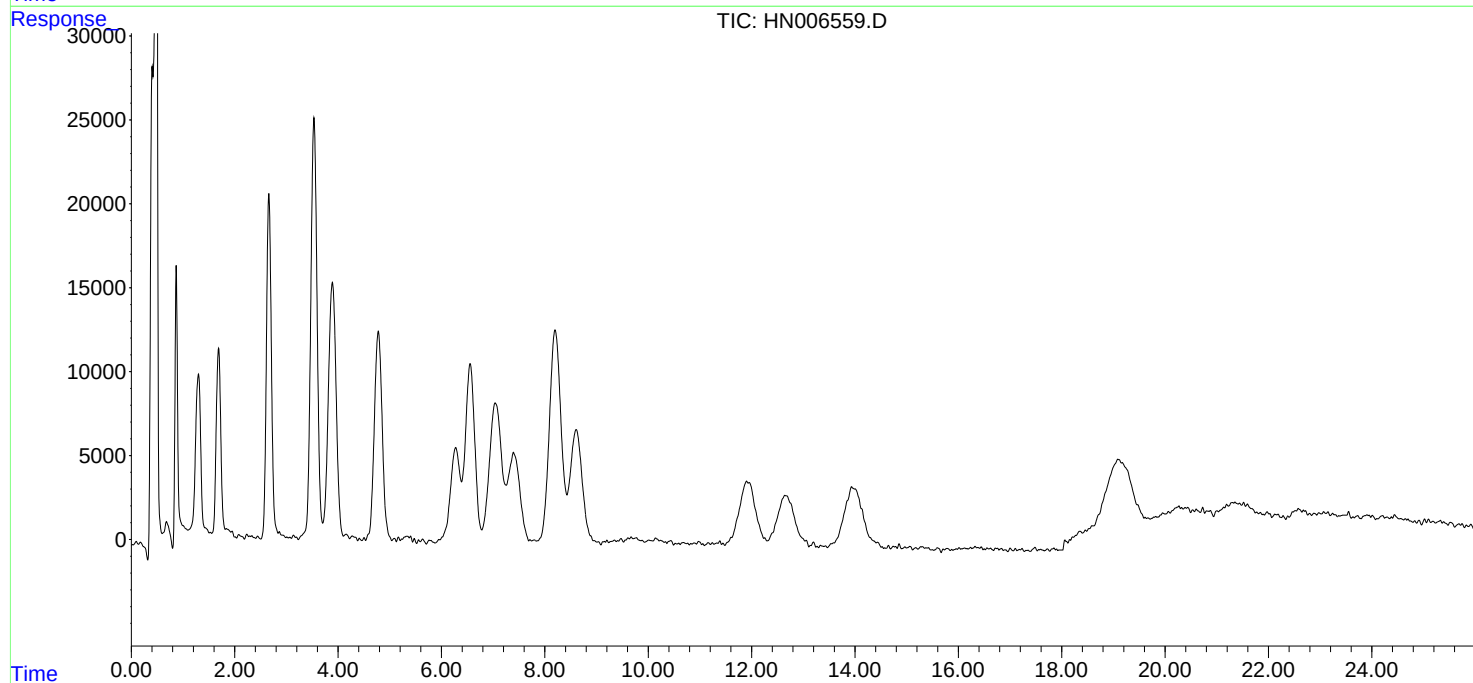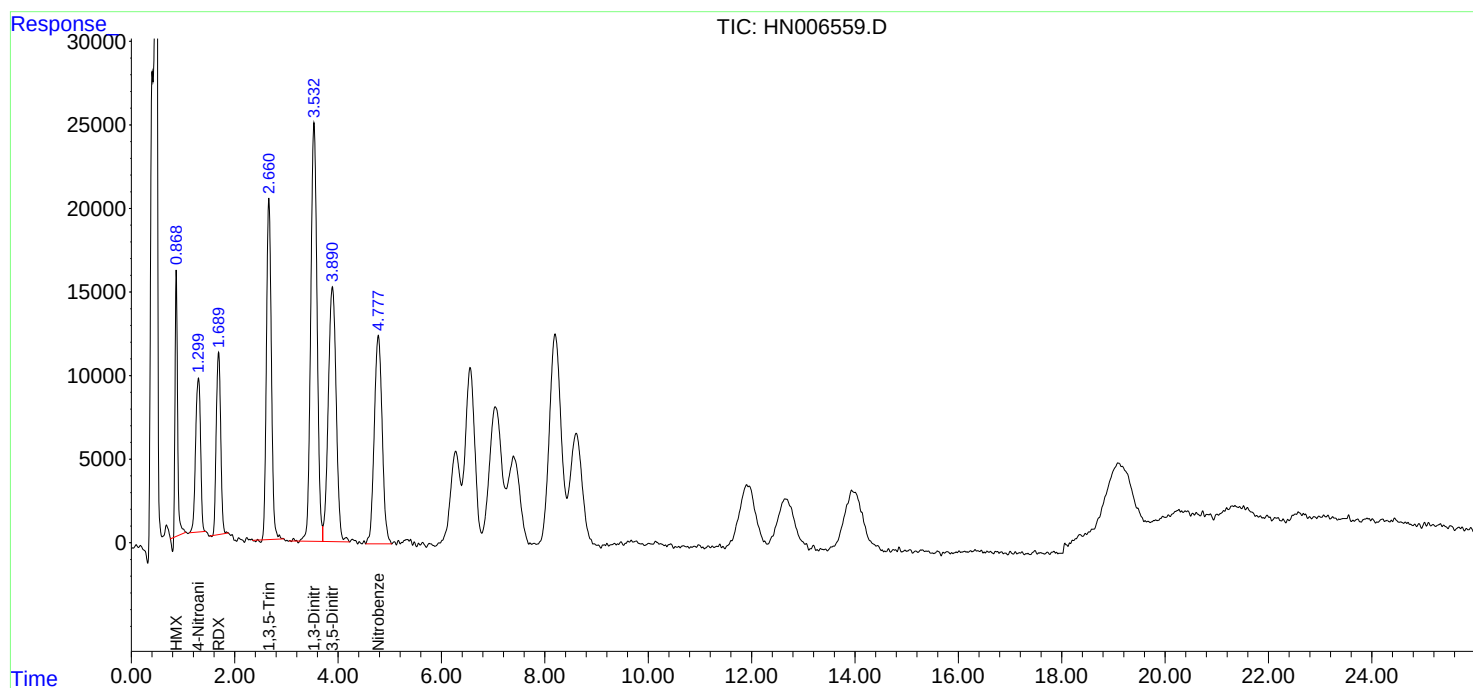


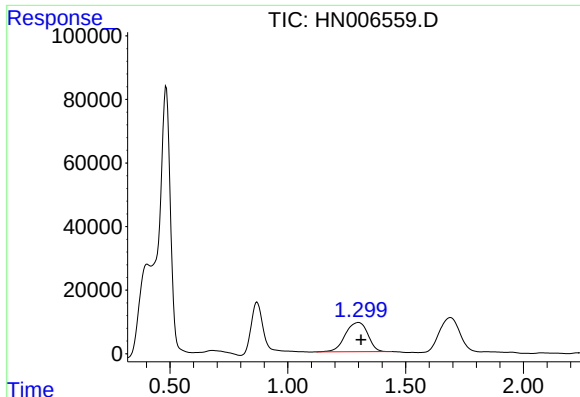

#1 4-Nitroaniline


R.T.: 1.300 min
Delta R.T.: -0.010 min
Response: 612796
Conc: 179.85 ug/L

Instrument :
HPLC_N
ClientSampleId :
PB79759BS

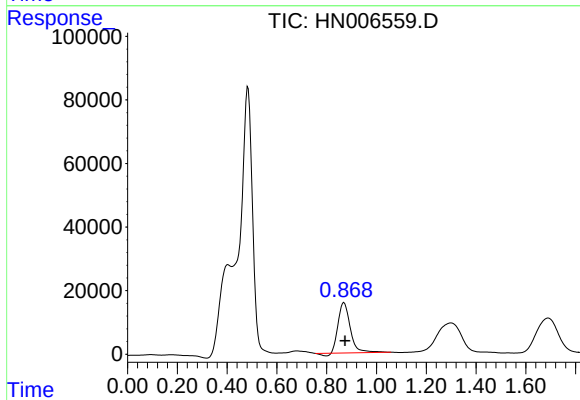


#2 HMX

R.T.: 0.870 min
Delta R.T.: -0.003 min
Response: 532194
Conc: 118.06 ug/L

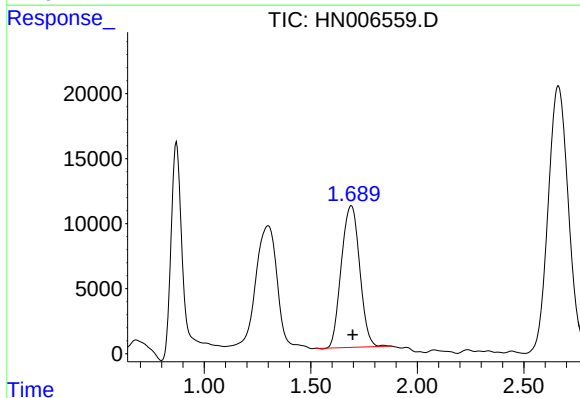


#3 RDX

R.T.: 1.690 min
Delta R.T.: -0.007 min
Response: 653695
Conc: 124.68 ug/L

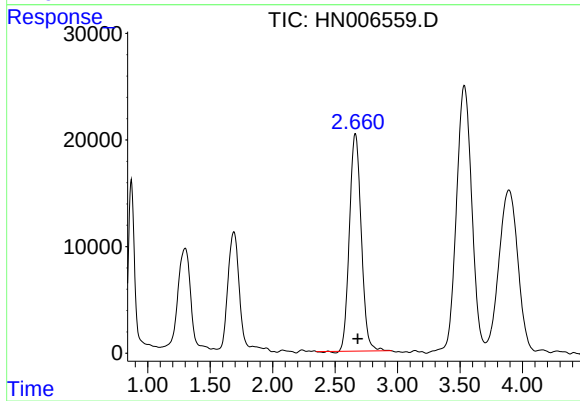

#4 1,3,5-Trinitrobenzene


R.T.: 2.662 min
Delta R.T.: -0.019 min
Response: 1340625
Conc: 124.88 ug/L

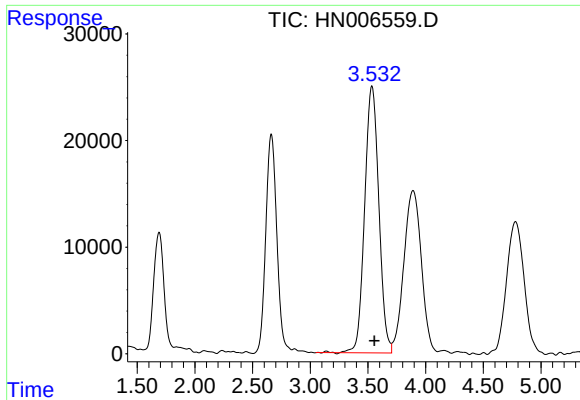

#5 1,3-Dinitrobenzene


R.T.: 3.534 min
Delta R.T.: -0.023 min
Response: 2138510
Conc: 131.08 ng/ml

Instrument :
HPLC_N
ClientSampleId :
PB79759BS

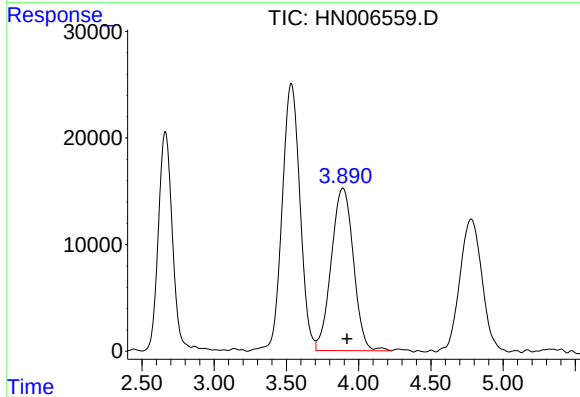

#6 3,5-Dinitroaniline

R.T.: 3.891 min
Delta R.T.: -0.029 min
Response: 1621322
Conc: 139.45 ug/L

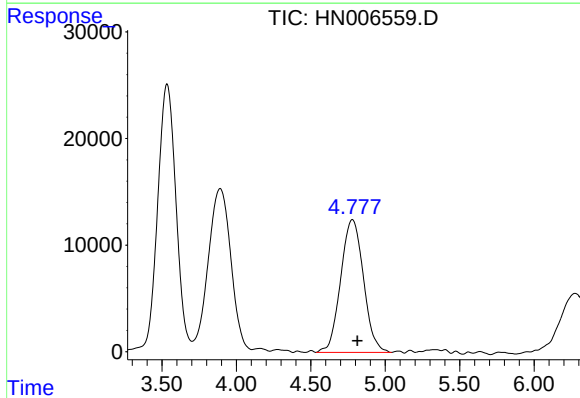

#7 Nitrobenzene

R.T.: 4.779 min
Delta R.T.: -0.034 min
Response: 1329118
Conc: 131.98 ug/L