

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN102314\
 Data File : HN006560.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 24-Oct-2014, 20:22
 Operator : HNP
 Sample : HSTDCCC0500
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDCCC0500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 02:19:57 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
 Quant Title :
 QLast Update : Mon Mar 09 14:56:25 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.303	1551134	455.252 ug/L
Target Compounds			
2) T HMX	0.871	2043396	453.285 ug/L
3) T RDX	1.687	2725571	519.857 ug/L
4) T 1,3,5-Trinitrobenzene	2.655	5567440	518.599 ug/L
5) T 1,3-Dinitrobenzene	3.523	8423476	516.315 ng/ml
6) T 3,5-Dinitroaniline	3.877	6062265	521.403 ug/L
7) T Nitrobenzene	4.760f	5097629	506.184 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN102314\
Data File : HN006560.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 24-Oct-2014, 20:22
Operator : HNP
Sample : HSTDCCC0500
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 02:19:57 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Quant Title :
QLast Update : Mon Mar 09 14:56:25 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

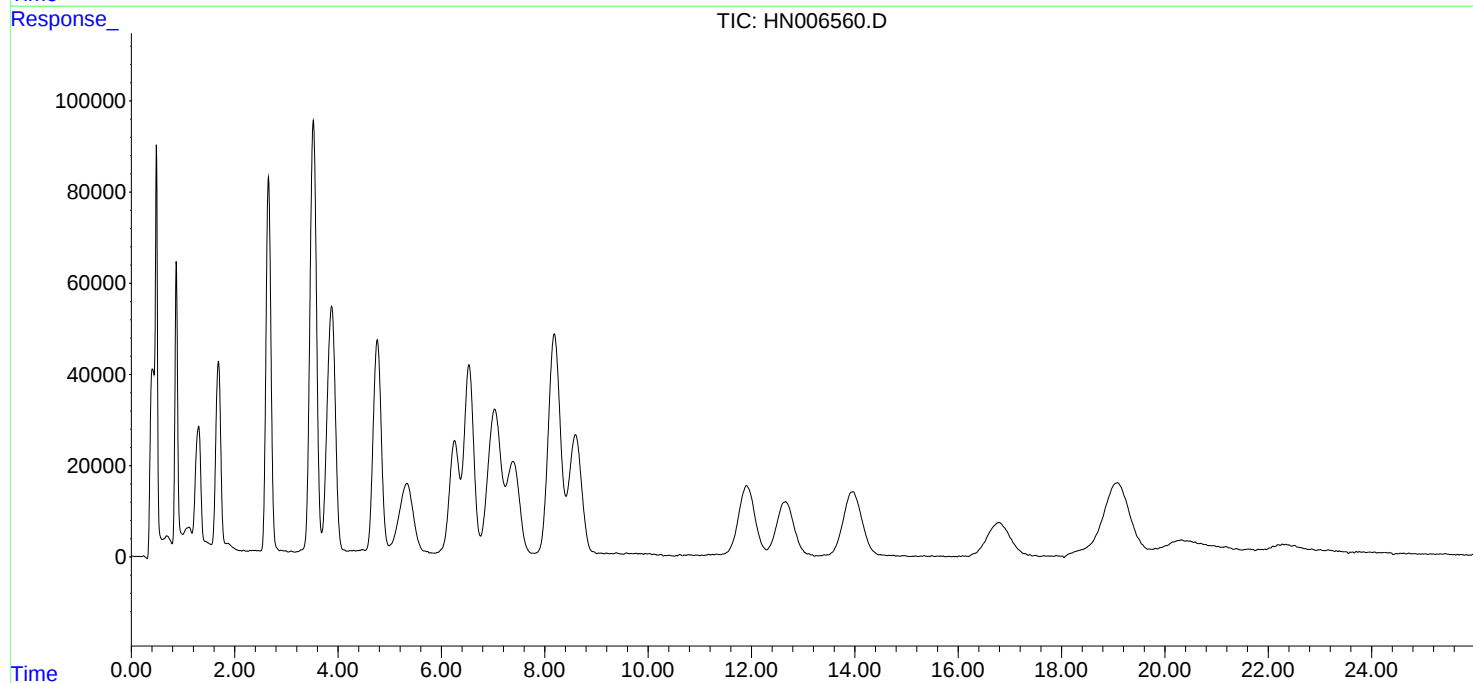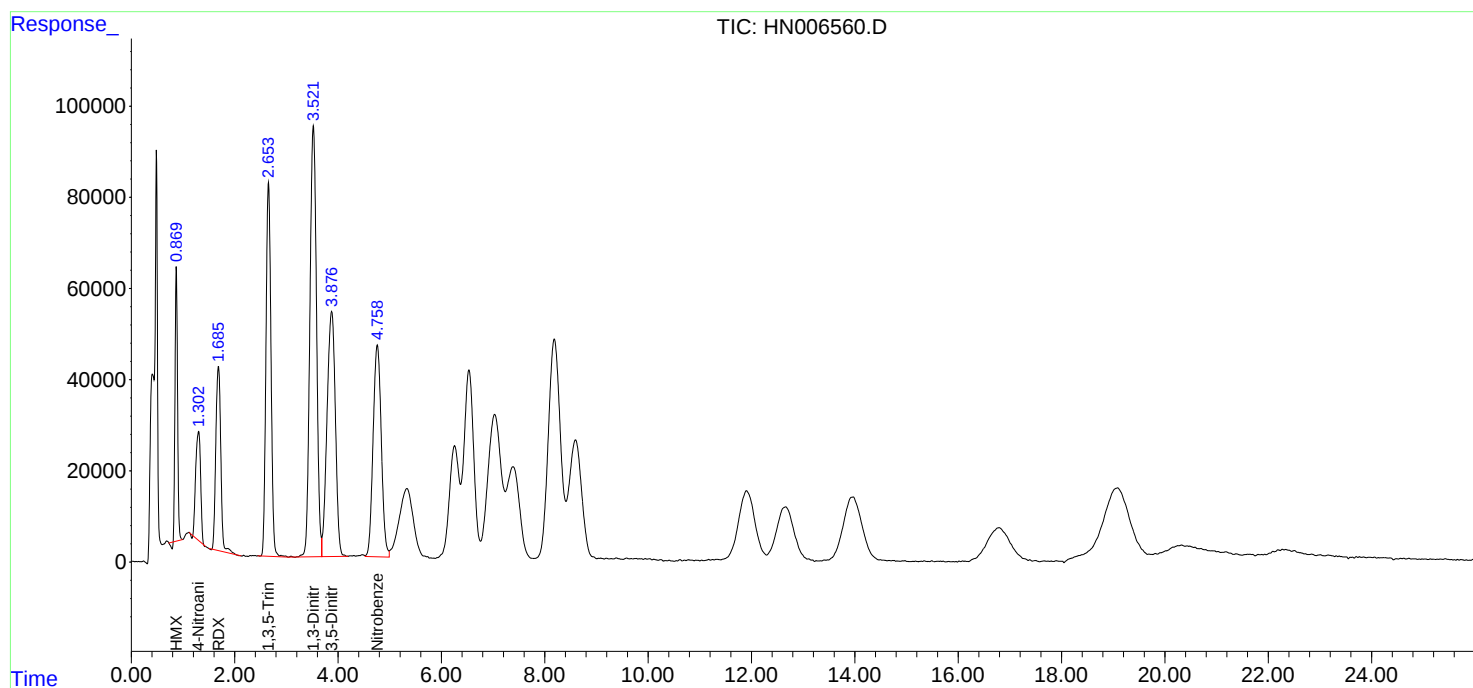


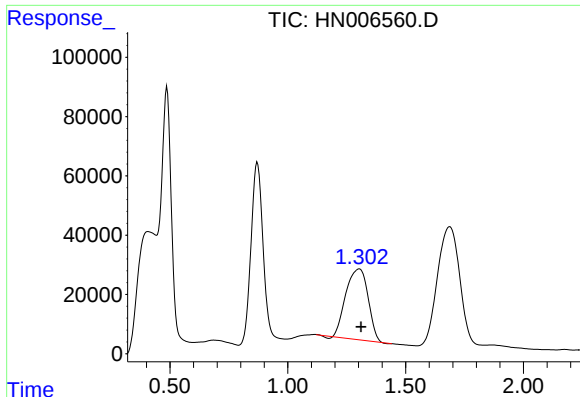

#1 4-Nitroaniline


R.T.: 1.303 min
Delta R.T.: -0.007 min
Response: 1551134
Conc: 455.25 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

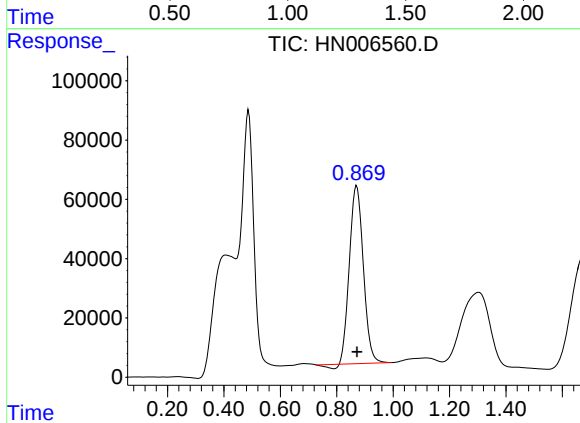


#2 HMX

R.T.: 0.871 min
Delta R.T.: -0.002 min
Response: 2043396
Conc: 453.28 ug/L

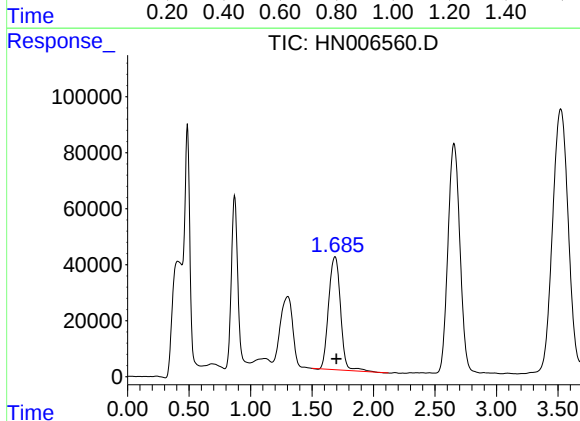


#3 RDX

R.T.: 1.687 min
Delta R.T.: -0.010 min
Response: 2725571
Conc: 519.86 ug/L

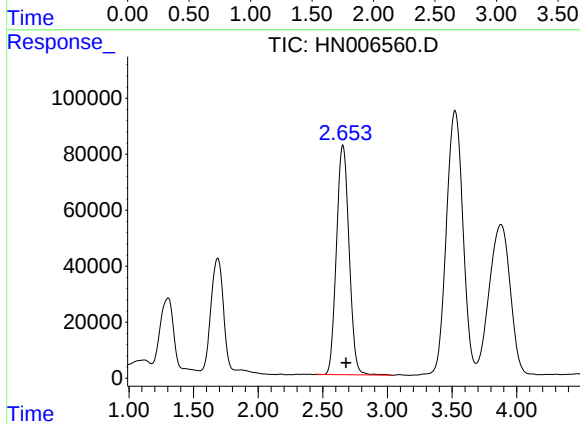

#4 1,3,5-Trinitrobenzene


R.T.: 2.655 min
Delta R.T.: -0.026 min
Response: 5567440
Conc: 518.60 ug/L

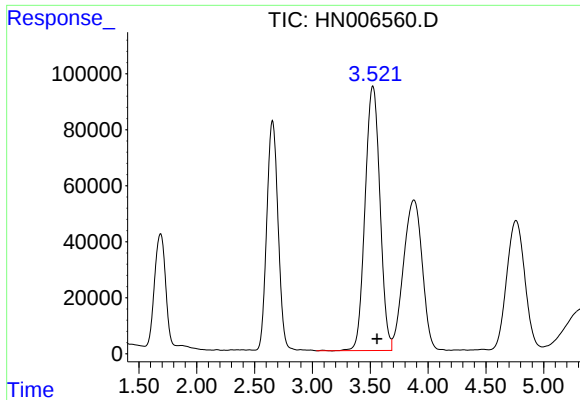

#5 1,3-Dinitrobenzene


R.T.: 3.523 min
Delta R.T.: -0.035 min
Response: 8423476
Conc: 516.31 ng/ml

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

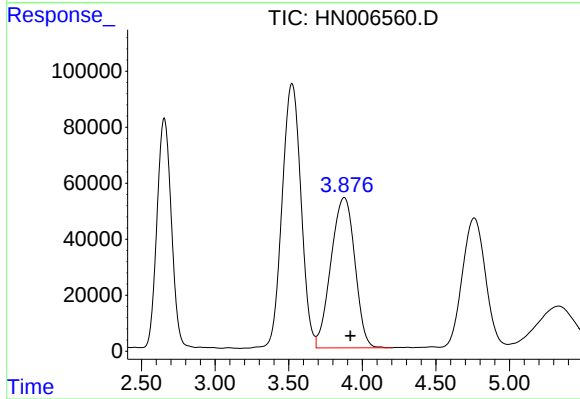

#6 3,5-Dinitroaniline

R.T.: 3.877 min
Delta R.T.: -0.043 min
Response: 6062265
Conc: 521.40 ug/L

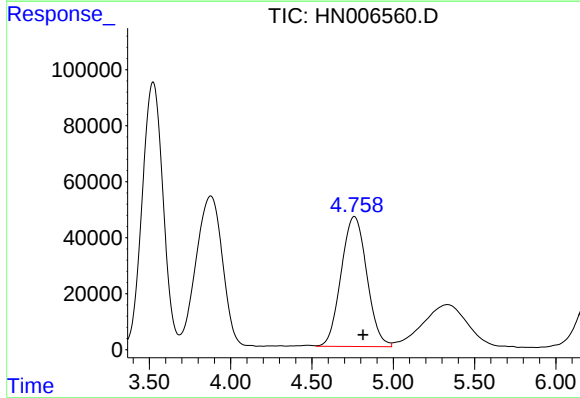

#7 Nitrobenzene

R.T.: 4.760 min
Delta R.T.: -0.053 min
Response: 5097629
Conc: 506.18 ug/L