

Data Path : Z:\HPCHEM1\HPLC\_N\Data\HN102314\  
Data File : HN006570.D  
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
Acq On : 24-Oct-2014, 22:38  
Operator : HNP  
Sample : F4322-07  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
HPLC\_N  
ClientSampleId :  
YS19-SS17-1014

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 11 02:29:53 2015  
Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN1016NG.M  
Quant Title :  
QLast Update : Fri Oct 17 04:15:53 2014  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

| Compound                    | R.T. | Response | Conc Units |
|-----------------------------|------|----------|------------|
| -----                       |      |          |            |
| System Monitoring Compounds |      |          |            |
| Target Compounds            |      |          |            |
| -----                       |      |          |            |

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC\_N\Data\HN102314\  
Data File : HN006570.D  
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
Acq On : 24-Oct-2014, 22:38  
Operator : HNP  
Sample : F4322-07  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
HPLC\_N  
ClientSampleId :  
YS19-SS17-1014

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 11 02:29:53 2015  
Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN1016NG.M  
Quant Title :  
QLast Update : Fri Oct 17 04:15:53 2014  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

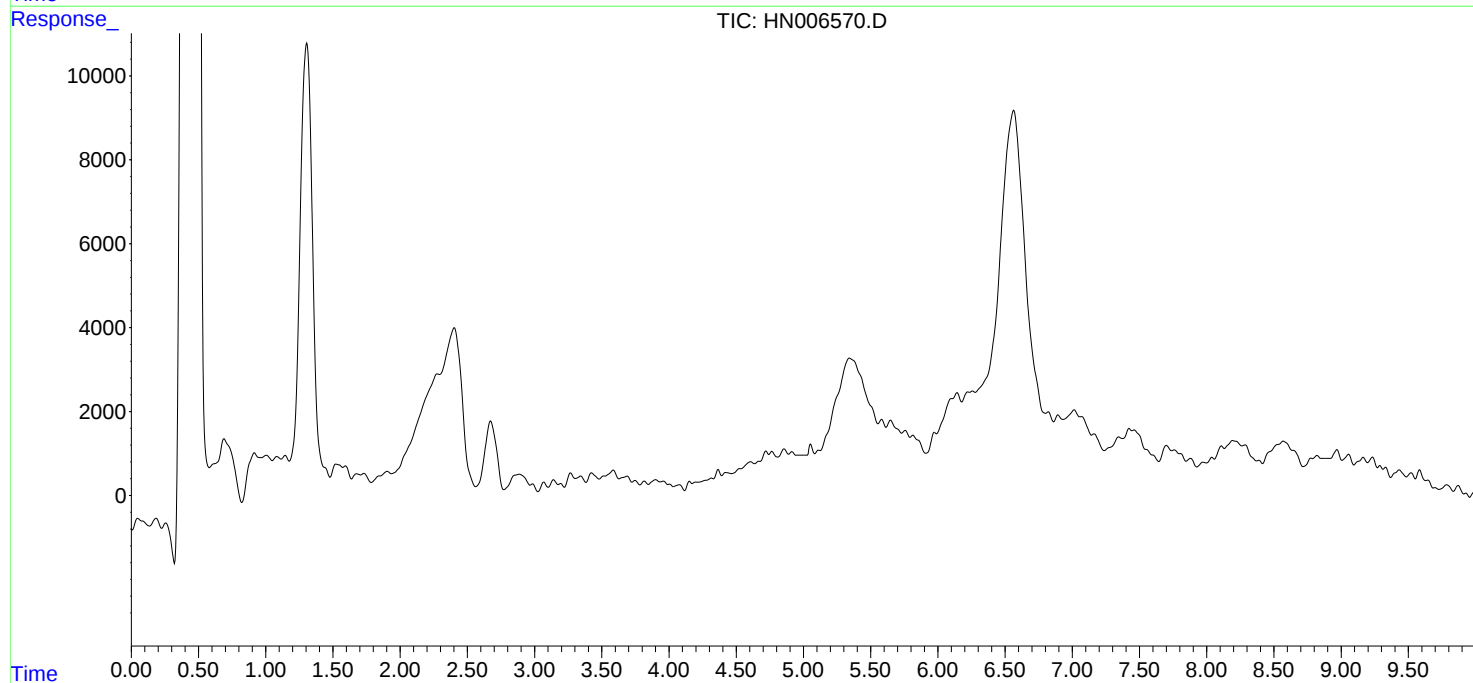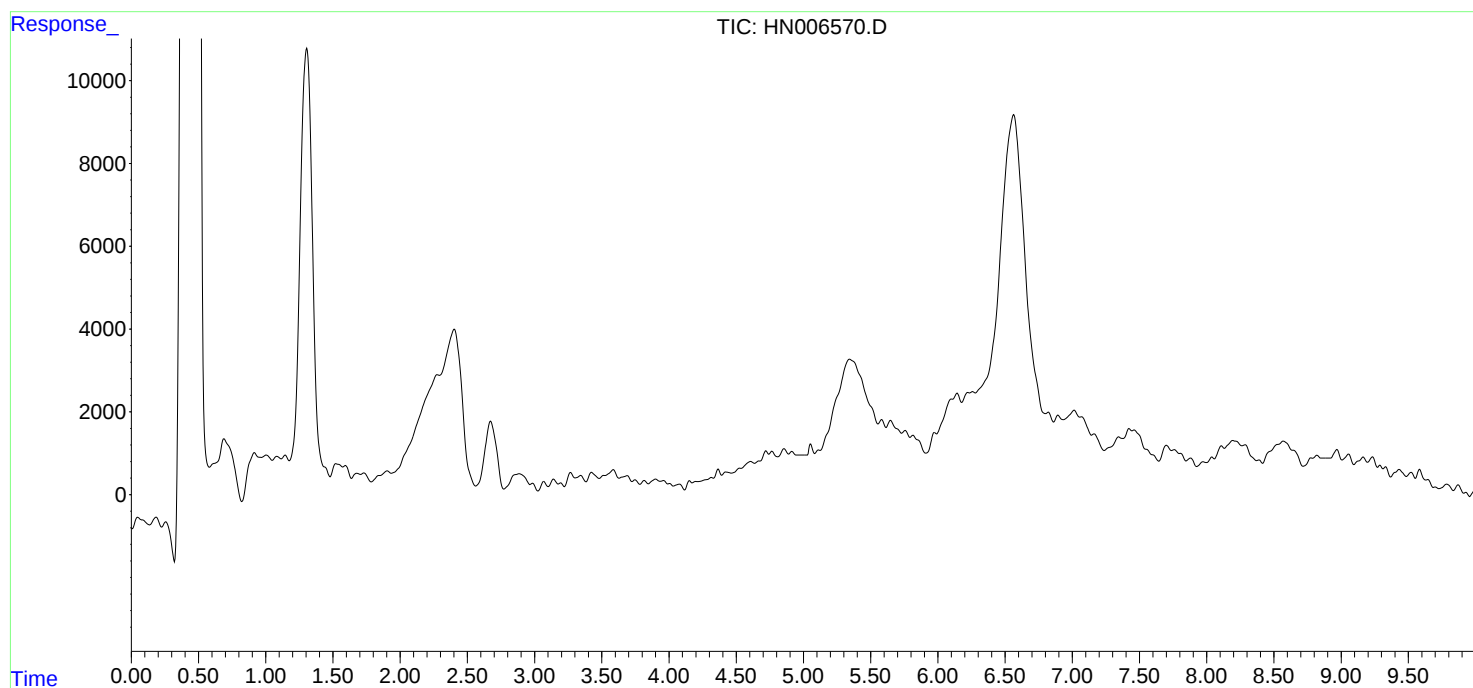

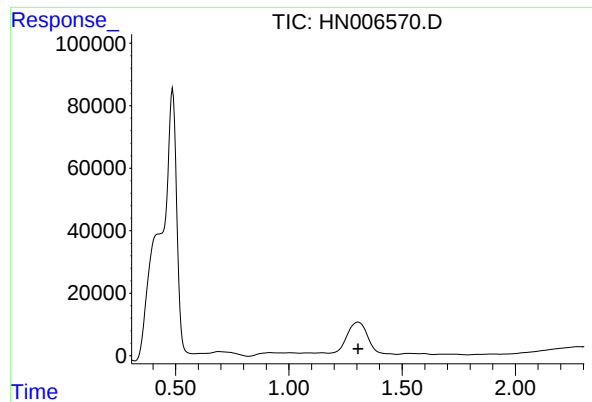

#1 4-Nitroaniline

R.T.: 0.000 min

Exp R.T. : 1.305 min

Response: 0

Conc: N.D.

Instrument :  
HPLC\_N  
ClientSampleId :  
YS19-SS17-1014