

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN102314\
 Data File : HN006505.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 23-Oct-2014, 18:41
 Operator : HNP
 Sample : F4325-03
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 YS19-SB19-1014MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 15:39:24 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\methods\HN100214.M
 Quant Title :
 QLast Update : Thu Mar 05 14:55:56 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.303	596789	175.156 ug/L
Target Compounds			
2) T HMX	0.872	495837	109.991 ug/L
3) T RDX	1.692f	685714	130.789 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN102314\
Data File : HN006505.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 23-Oct-2014, 18:41
Operator : HNP
Sample : F4325-03
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
YS19-SB19-1014MS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 15:39:24 2015
Quant Method : Z:\HPCHEM1\HPLC_N\methods\HN100214.M
Quant Title :
QLast Update : Thu Mar 05 14:55:56 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

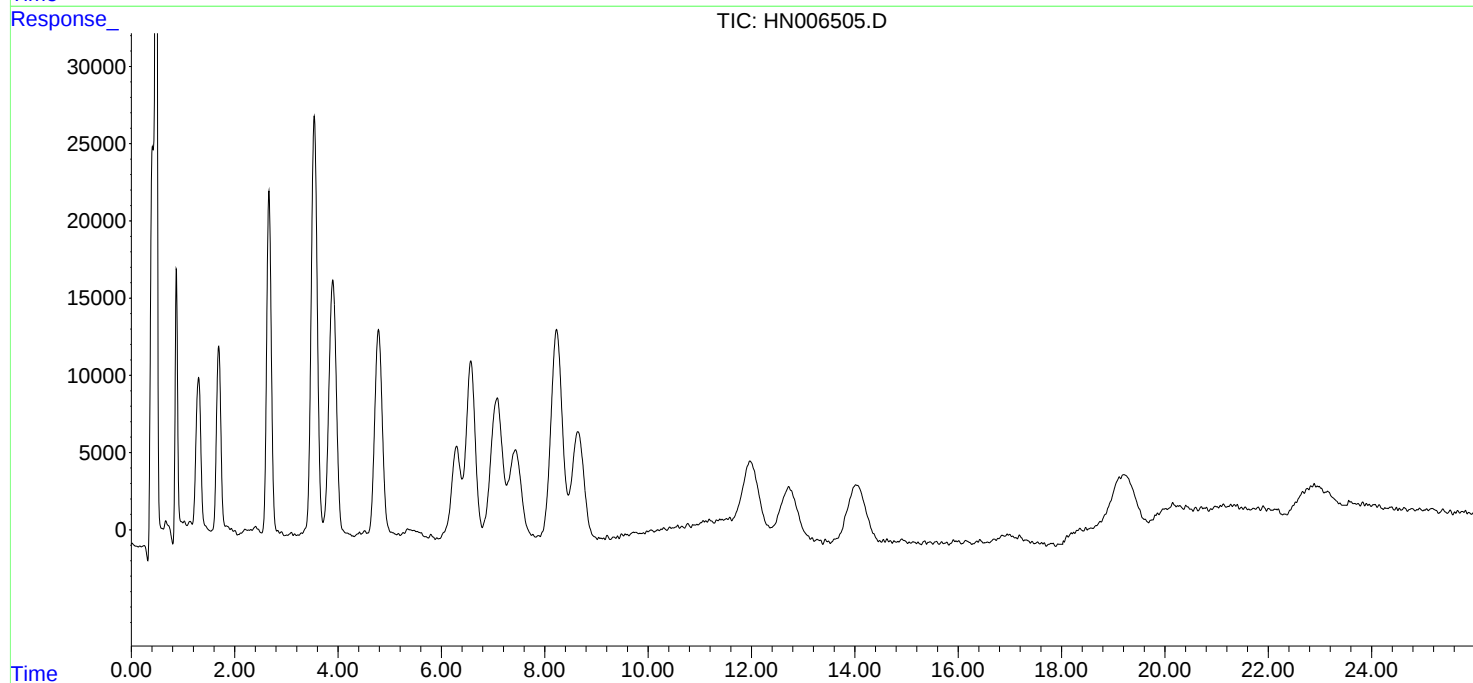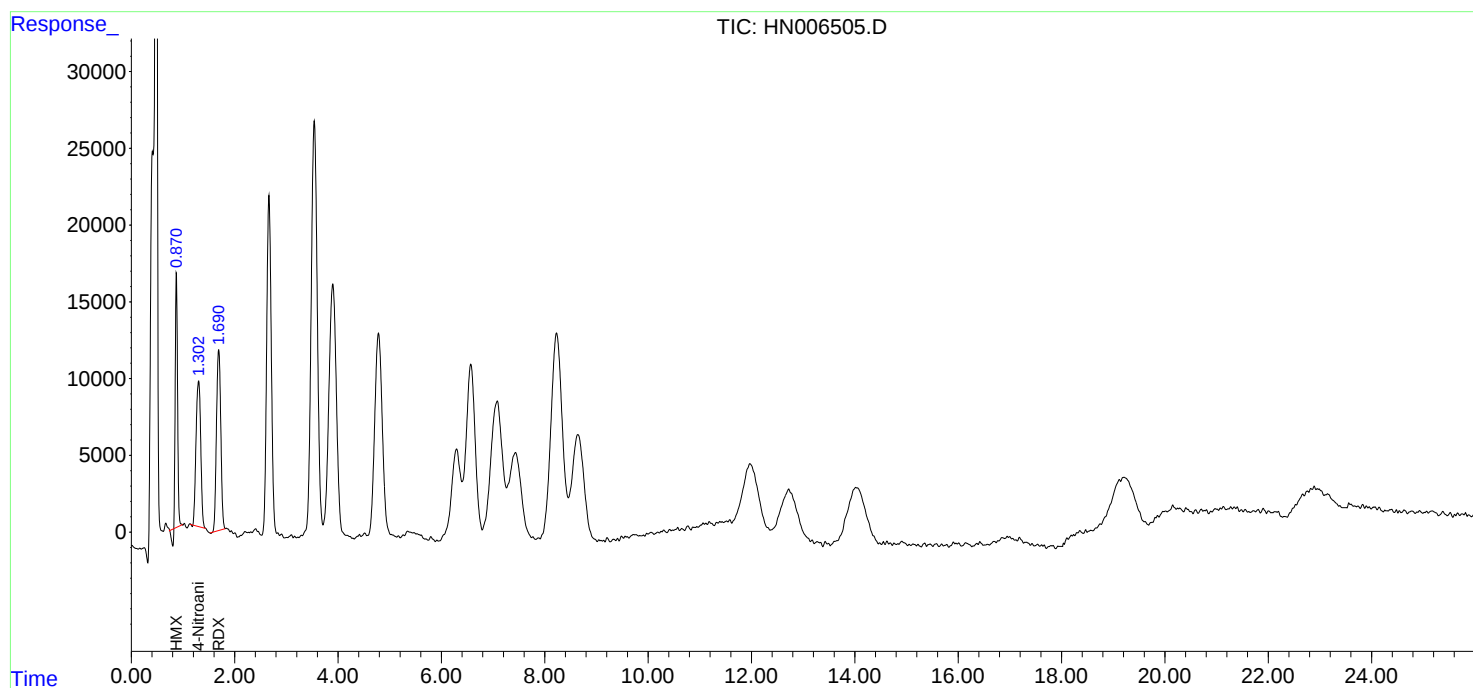


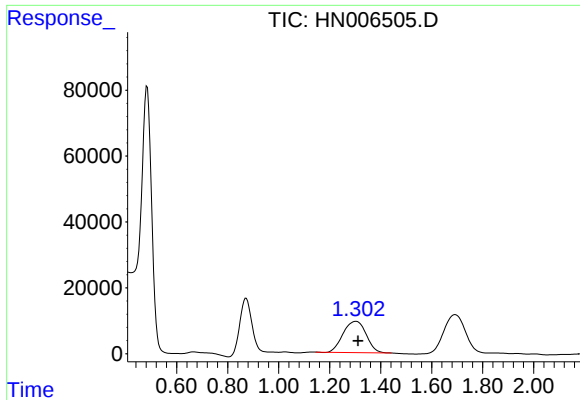

#1 4-Nitroaniline


R.T.: 1.303 min
Delta R.T.: -0.008 min
Response: 596789
Conc: 175.16 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-SB19-1014MS

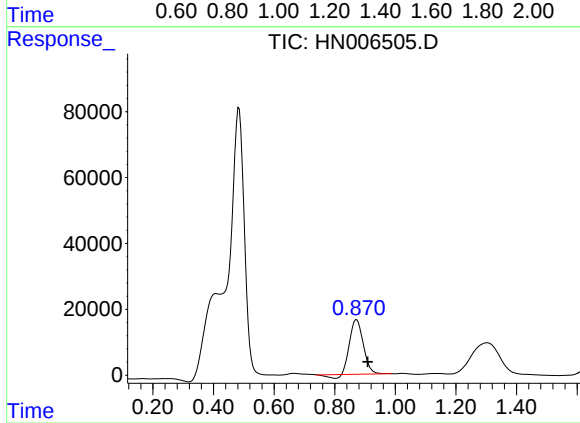

#2 HMX

R.T.: 0.872 min
Delta R.T.: -0.037 min
Response: 495837
Conc: 109.99 ug/L

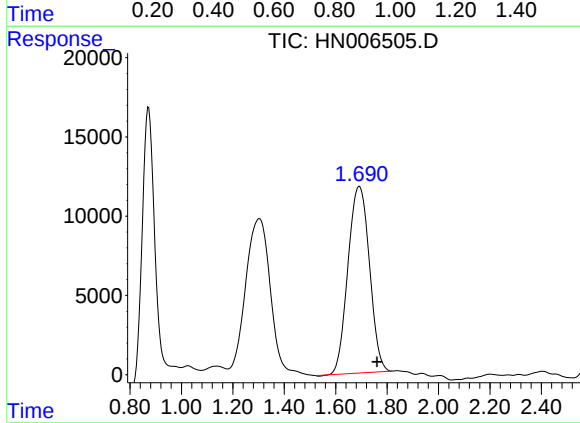

#3 RDX

R.T.: 1.692 min
Delta R.T.: -0.069 min
Response: 685714
Conc: 130.79 ug/L