

Data Path : Z:\HPCHEM1\HPLC\_N\Data\HN102314\  
Data File : HN006605.D  
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
Acq On : 25-Oct-2014, 05:38  
Operator : HNP  
Sample : HSTDCCC005  
Misc :  
ALS Vial : 91 Sample Multiplier: 1

Instrument :  
HPLC\_N  
ClientSampleId :  
HSTDCCC005

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 27 01:27:12 2014  
Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN1016NG.M  
Quant Title :  
QLast Update : Fri Oct 17 04:15:53 2014  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

| Compound                    | R.T.  | Response | Conc Units  |
|-----------------------------|-------|----------|-------------|
| -----                       |       |          |             |
| System Monitoring Compounds |       |          |             |
| 1) S 4-Nitroaniline         | 1.310 | 19894330 | 5.009 ng/ul |
|                             |       |          |             |
| Target Compounds            |       |          |             |
| 2) T Nitroglycerin          | 6.066 | 38233371 | 4.992 ng/ul |
| -----                       |       |          |             |

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC\_N\Data\HN102314\  
Data File : HN006605.D  
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
Acq On : 25-Oct-2014, 05:38  
Operator : HNP  
Sample : HSTDCCC005  
Misc :  
ALS Vial : 91 Sample Multiplier: 1

Instrument :  
HPLC\_N  
ClientSampleId :  
HSTDCCC005

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 27 01:27:12 2014  
Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN1016NG.M  
Quant Title :  
QLast Update : Fri Oct 17 04:15:53 2014  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

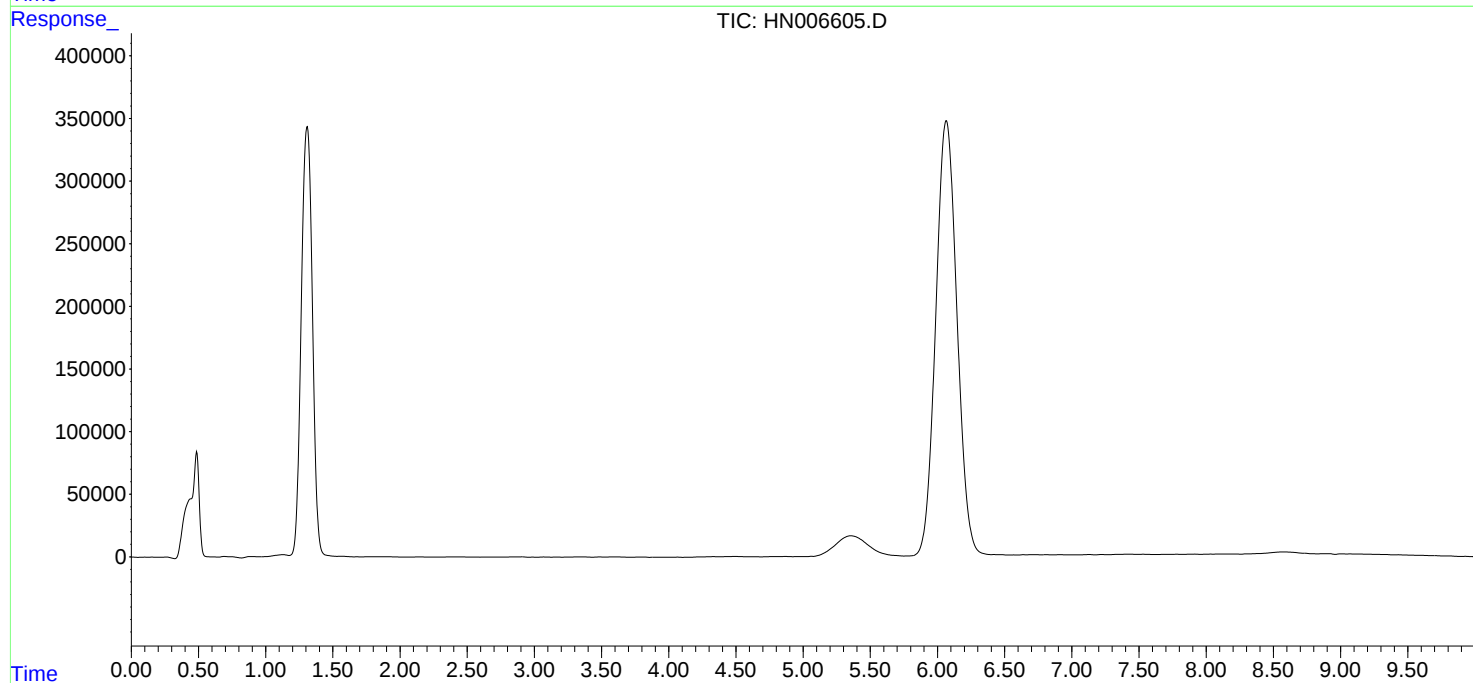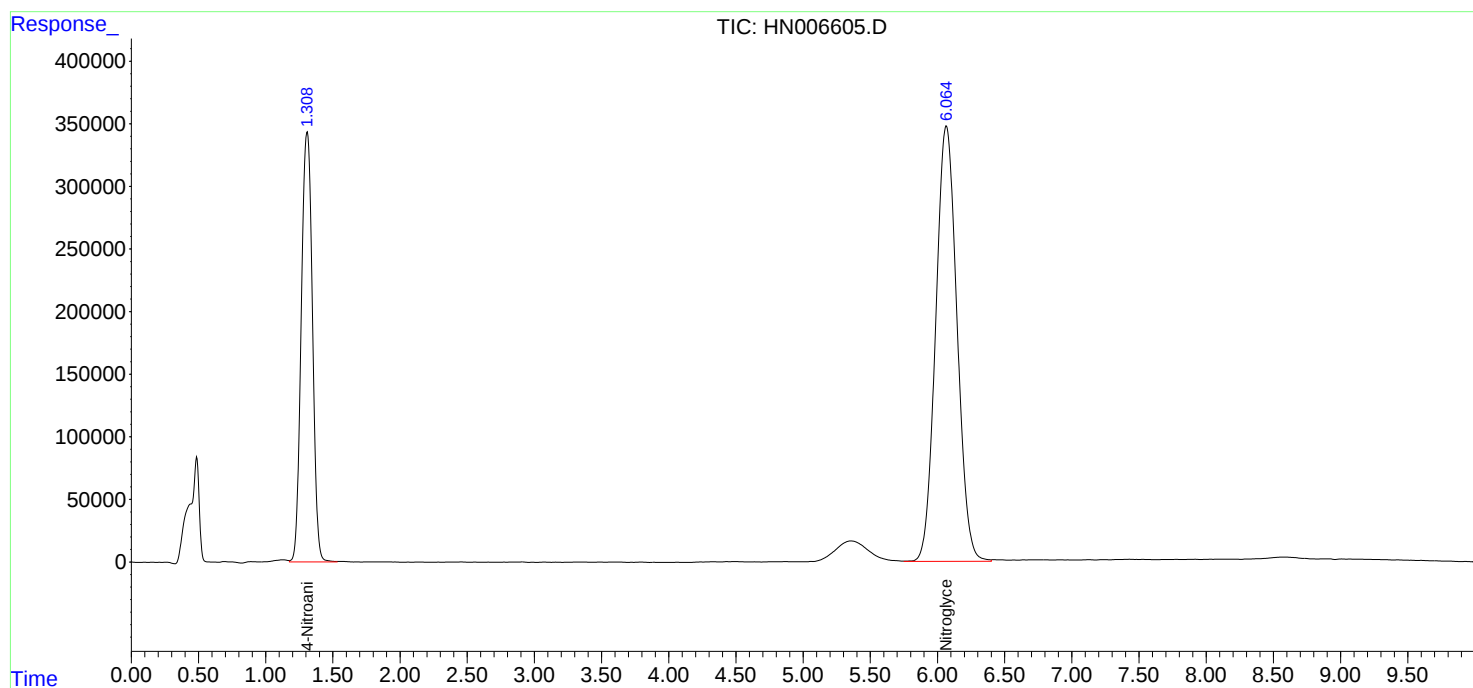


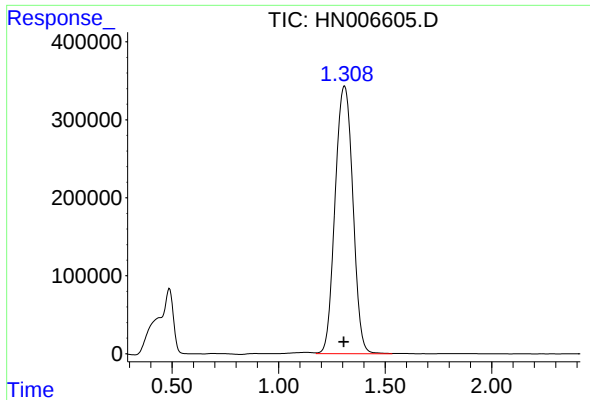

#1 4-Nitroaniline

R.T.: 1.310 min  
Delta R.T.: 0.004 min  
Response: 19894330  
Conc: 5.01 ng/ul

Instrument :  
HPLC\_N  
ClientSampleId :  
HSTDCCC005

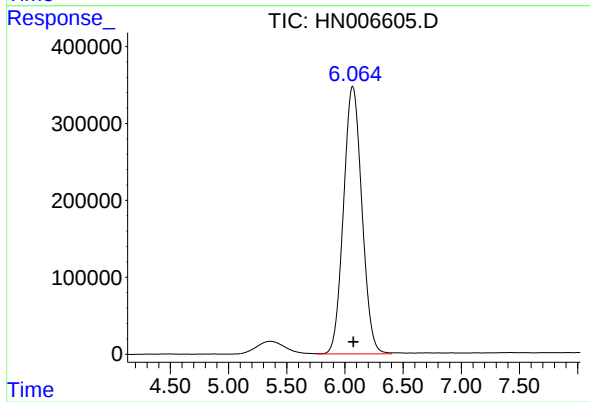

#2 Nitroglycerin

R.T.: 6.066 min  
Delta R.T.: -0.008 min  
Response: 38233371  
Conc: 4.99 ng/ul