

Signal #1 : Z:\HPCHEM1\HPLC\_N\DATA\HN102314\HN006499.D\VWD1A.CH Vial: 22  
Signal #2 : Z:\HPCHEM1\HPLC\_N\DATA\HN102314\HN006499.D\VWD1A.CH  
Acq On : 23-Oct-2014, 15:53 Operator: HNP  
Sample : F4337-07 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e  
Quant Time: Oct 27 2:04 2014 Quant Results File: HN100214.RES

Instrument :  
HPLC\_N  
ClientSampleId :  
YS19-SS24-1014

Manual Integrations  
APPROVED

ugo  
11/3/2014 11:45:30 AM

Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN100214.M  
Title :  
Last Update : Sat Oct 25 01:28:50 2014  
Response via : Initial Calibration  
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

| Compound                    | R.T. | Response | Conc Units     |
|-----------------------------|------|----------|----------------|
| -----                       |      |          |                |
| System Monitoring Compounds |      |          |                |
| 1) S 4-Nitroaniline         | 1.34 | 547169   | 137.669 ug/L m |

Target Compounds

-----  
Analyst Signature:\_\_\_\_\_ Analyst Name:\_\_\_\_\_ Date:\_\_\_\_\_

-----REASONS FOR MANUAL INTEGRATIONS-----

\_\_\_Poor resolution of peaks exhibited on chromatogram.Compound #:\_\_\_\_\_

\_\_\_Peak Integrated by software incorrectly.Compound #:\_\_\_\_\_

\_\_\_OTHER:\_\_\_\_\_Compound #:\_\_\_\_\_

(f)=RT Delta > 1/2 Window (m)=manual int.

HN006499.D HN100214.M Sat Nov 08 00:16:14 2014

## Quantitation Report

Signal #1 : Z:\HPCHEM1\HPLC\_N\DATA\HN102314\HN006499.D\VWD1A.CH Vial: 22  
Signal #2 : Z:\HPCHEM1\HPLC\_N\DATA\HN102314\HN006499.D\VWD1A.CH  
Acq On : 23-Oct-2014, 15:53 Operator: HNP  
Sample : F4337-07 Inst : G1314A  
Misc : Multiplr: 1.00  
IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e  
Quant Time: Oct 27 2:04 2014 Quant Results File: HN100214.RES



Instrument :  
HPLC\_N  
ClientSampleId :  
YS19-SS24-1014


Manual Integrations  
APPROVED

ugo  
11/3/2014 11:45:30 AM

Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN100214.M  
Title :  
Last Update : Sat Oct 25 01:28:50 2014  
Response via : Multiple Level Calibration  
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

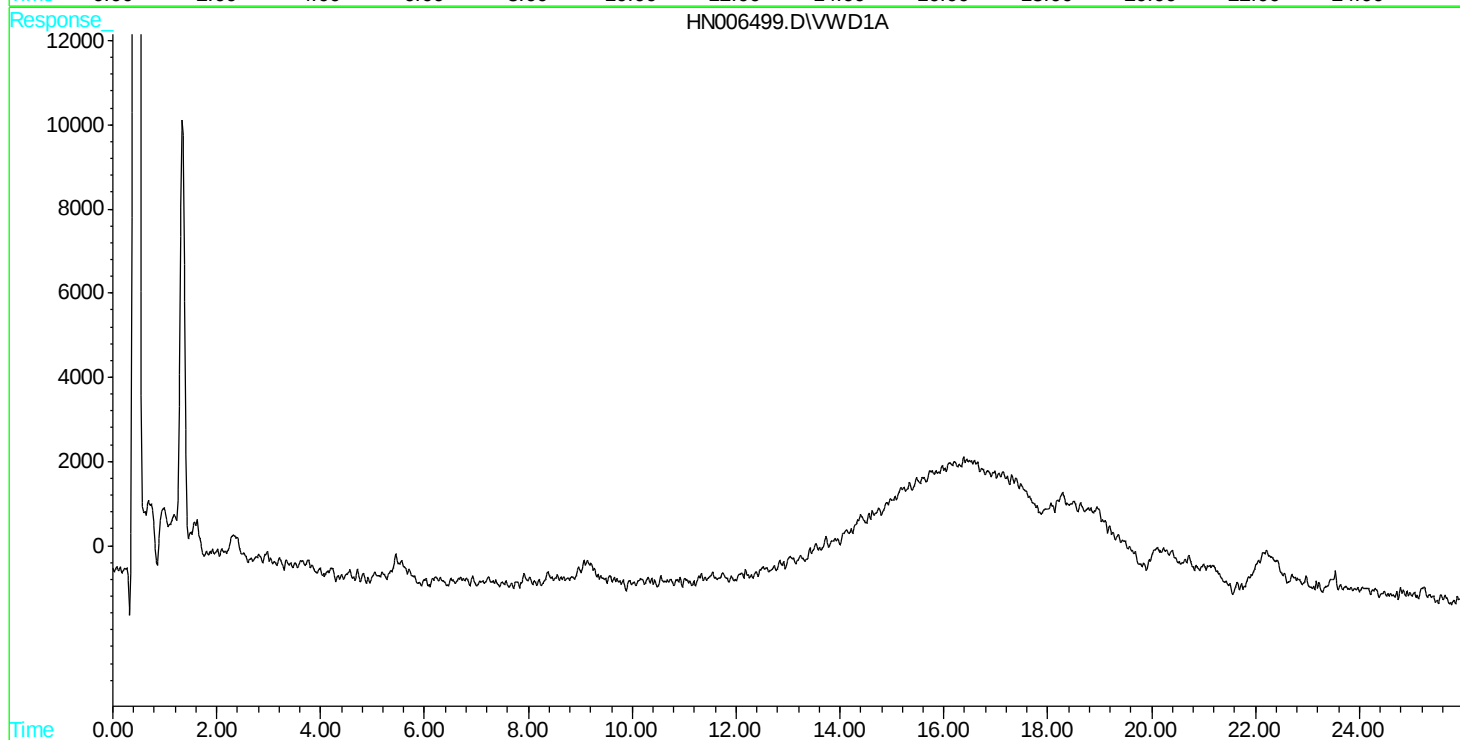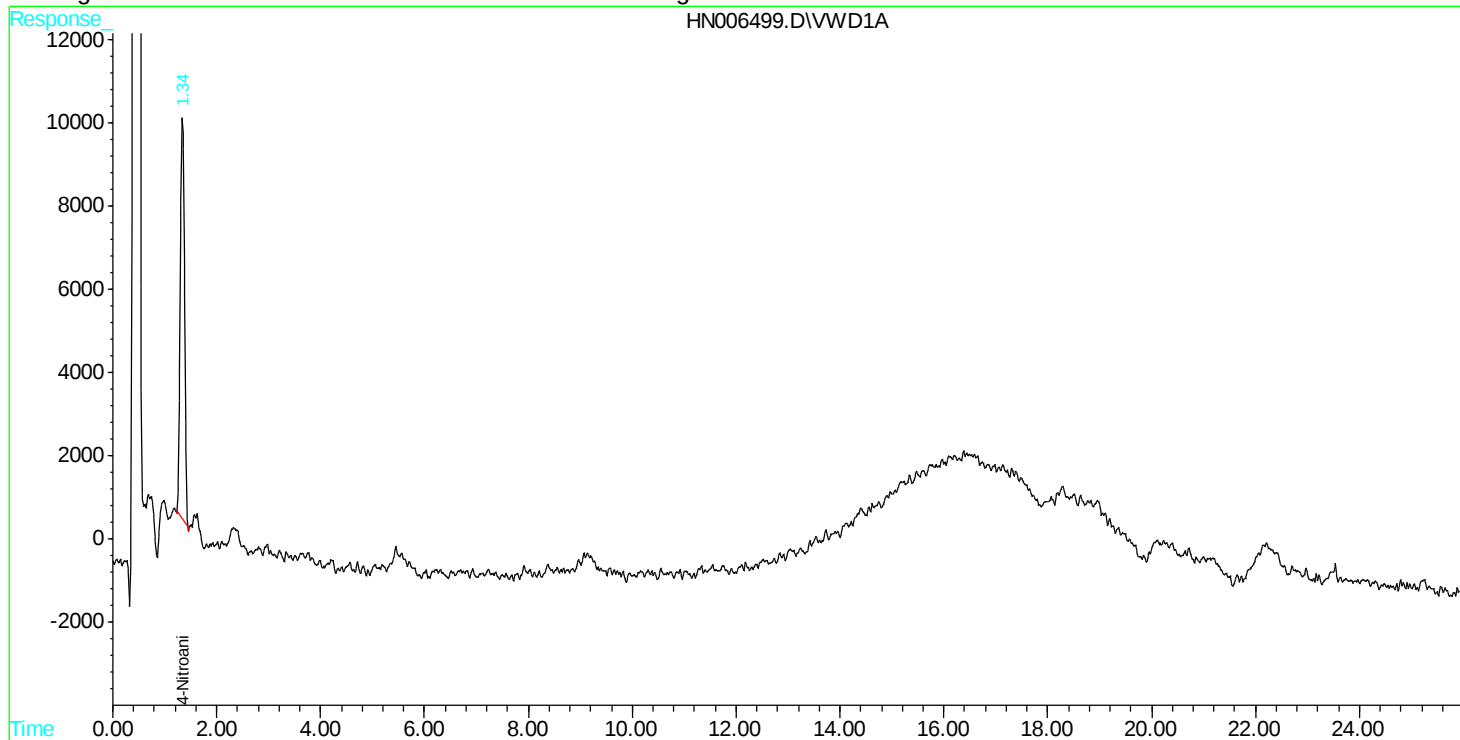

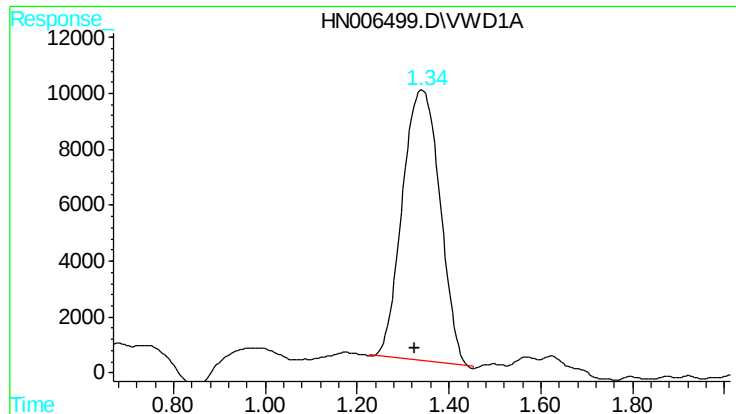

#1 4-Nitroaniline

R.T.: 1.340 min  
Delta R.T.: 0.013 min  
Response: 547169  
Conc: 137.67 ug/L m

Instrument :  
HPLC\_N  
ClientSampleId :  
YS19-SS24-1014

Manual Integrations  
APPROVED

ugo  
11/3/2014 11:45:30 AM