

Signal #1 : Z:\HPCHEM1\HPLC\_N\DATA\HN102314\HN006521.D\VWD1A.CH Vial: 42  
 Signal #2 : Z:\HPCHEM1\HPLC\_N\DATA\HN102314\HN006521.D\VWD1A.CH  
 Acq On : 24-Oct-2014, 02:09 Operator: HNP  
 Sample : F4325-19 Inst : G1314A  
 Misc : Multiplr: 1.00  
 IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e  
 Quant Time: Oct 27 3:00 2014 Quant Results File: HN100214.RES

Instrument :  
 HPLC\_N  
 ClientSampleId :  
 YS19-SS20-1014

Manual Integrations  
 APPROVED

ugo  
 11/3/2014 11:47:22 AM

Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN100214.M  
 Title :  
 Last Update : Sat Oct 25 01:28:50 2014  
 Response via : Initial Calibration  
 DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul  
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

| Compound                    | R.T. | Response | Conc Units     |
|-----------------------------|------|----------|----------------|
| -----                       |      |          |                |
| System Monitoring Compounds |      |          |                |
| 1) S 4-Nitroaniline         | 1.30 | 612978   | 154.227 ug/L m |

Target Compounds

-----  
 Analyst Signature:\_\_\_\_\_ Analyst Name:\_\_\_\_\_ Date:\_\_\_\_\_

-----REASONS FOR MANUAL INTEGRATIONS-----

\_\_\_Poor resolution of peaks exhibited on chromatogram.Compound #:\_\_\_\_\_

\_\_\_Peak Integrated by software incorrectly.Compound #:\_\_\_\_\_

\_\_\_OTHER:\_\_\_\_\_Compound #:\_\_\_\_\_

(f)=RT Delta > 1/2 Window (m)=manual int.

HN006521.D HN100214.M Sat Nov 08 00:22:15 2014

# Quantitation Report

Signal #1 : Z:\HPCHEM1\HPLC\_N\DATA\HN102314\HN006521.D\VWD1A.CH Vial: 42  
 Signal #2 : Z:\HPCHEM1\HPLC\_N\DATA\HN102314\HN006521.D\VWD1A.CH  
 Acq On : 24-Oct-2014, 02:09 Operator: HNP  
 Sample : F4325-19 Inst : G1314A  
 Misc : Multiplr: 1.00  
 IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e  
 Quant Time: Oct 27 3:00 2014 Quant Results File: HN100214.RES



Instrument :  
 HPLC\_N  
 ClientSampleId :  
 YS19-SS20-1014


Manual Integrations  
 APPROVED

ugo  
 11/3/2014 11:47:22 AM

Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN100214.M  
 Title :  
 Last Update : Sat Oct 25 01:28:50 2014  
 Response via : Multiple Level Calibration  
 DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul  
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

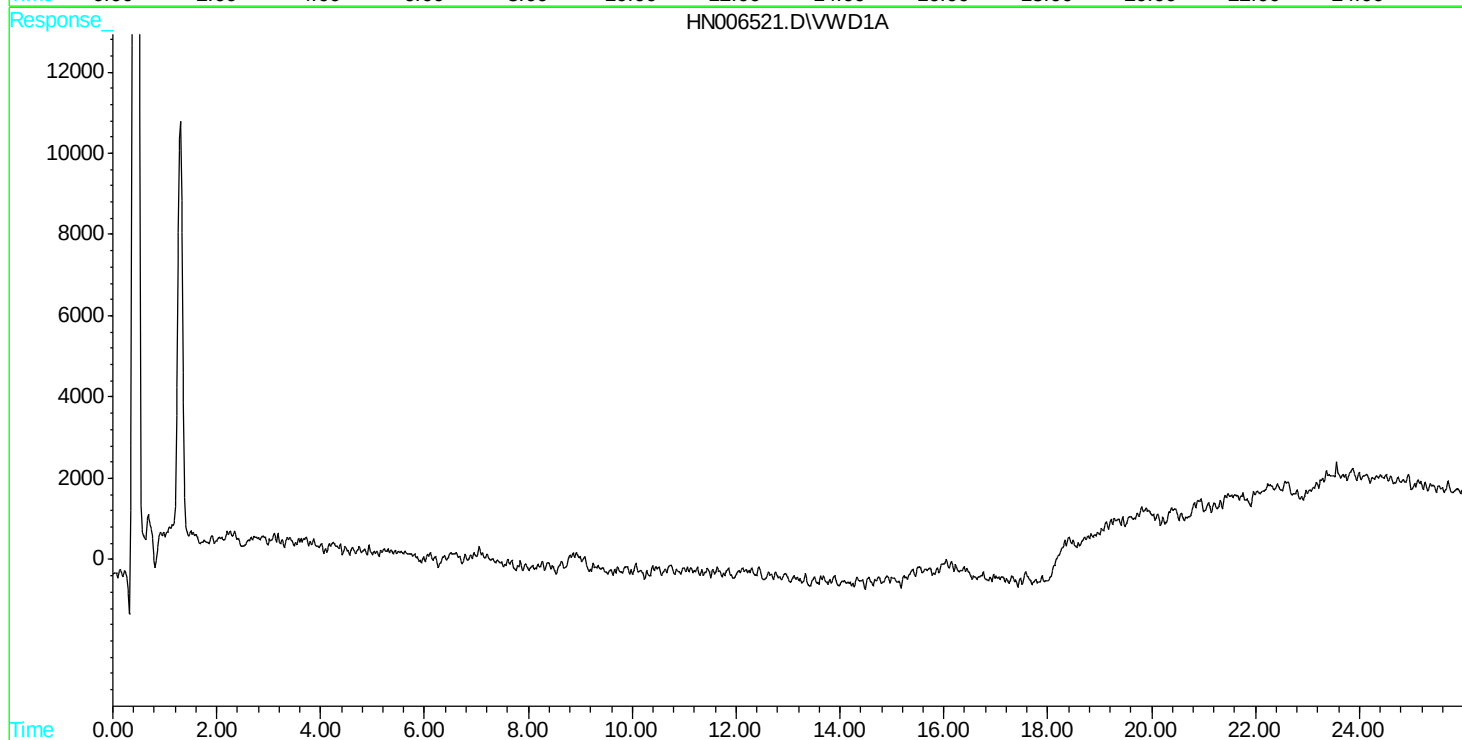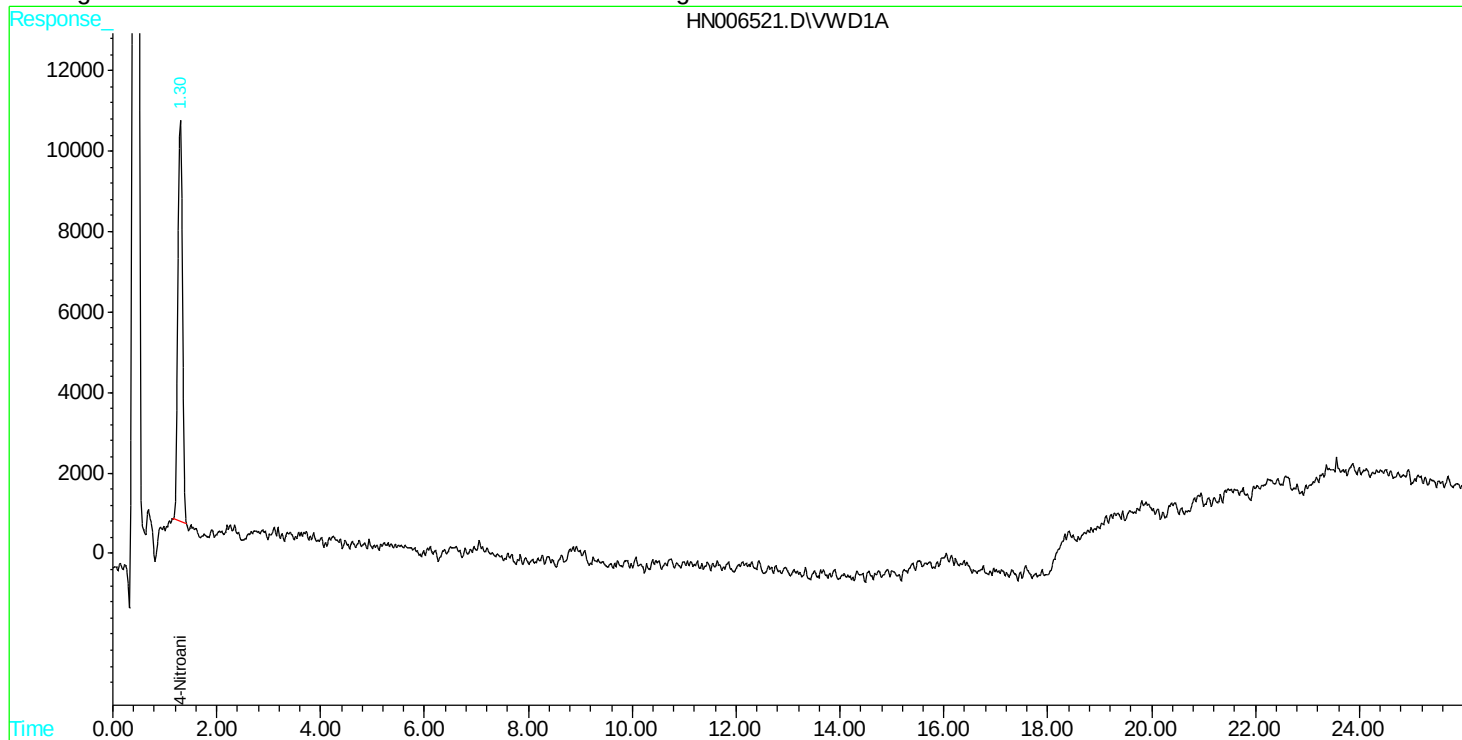

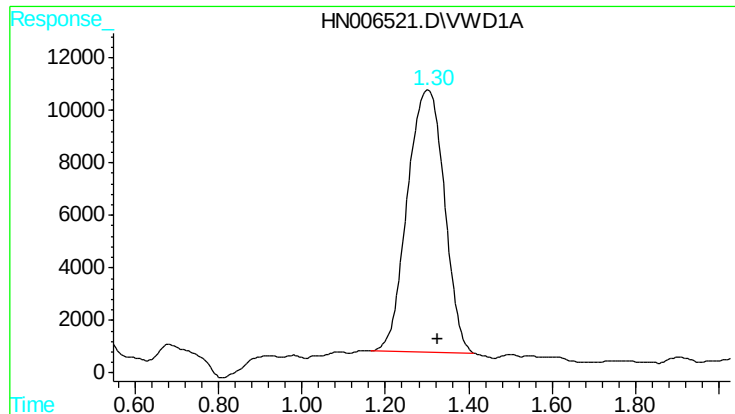

#1 4-Nitroaniline

R.T.: 1.301 min  
Delta R.T.: -0.026 min  
Response: 612978  
Conc: 154.23 ug/L m

Instrument :  
HPLC\_N  
ClientSampleId :  
YS19-SS20-1014

Manual Integrations  
APPROVED

ugo  
11/3/2014 11:47:22 AM