

Signal #1 : Z:\HPCHEM1\HPLC\_N\DATA\HN102314\HN006578.D\VWD1A.CH Vial: 17  
 Signal #2 : Z:\HPCHEM1\HPLC\_N\DATA\HN102314\HN006578.D\VWD1A.CH  
 Acq On : 25-Oct-2014, 00:14 Operator: HNP  
 Sample : F4337-02MSD Inst : G1314A  
 Misc : Multiplr: 1.00  
 IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e  
 Quant Time: Oct 27 0:19 2014 Quant Results File: HN1016NG.RES

Instrument :  
 HPLC\_N  
 ClientSampleId :  
 YS19-SB21-1014MSD

Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN1016NG.M  
 Title :  
 Last Update : Fri Oct 17 04:15:53 2014  
 Response via : Initial Calibration  
 DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul  
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

| Compound                    | R.T. | Response | Conc Units  |
|-----------------------------|------|----------|-------------|
| -----                       |      |          |             |
| System Monitoring Compounds |      |          |             |
| 1) S 4-Nitroaniline         | 1.30 | 599539   | 0.151 ng/ul |
| Target Compounds            |      |          |             |

-----  
 Analyst Signature:\_\_\_\_\_ Analyst Name:\_\_\_\_\_ Date:\_\_\_\_\_

-----REASONS FOR MANUAL INTEGRATIONS-----

\_\_\_Poor resolution of peaks exhibited on chromatogram.Compound #:\_\_\_\_\_

\_\_\_Peak Integrated by software incorrectly.Compound #:\_\_\_\_\_

\_\_\_OTHER:\_\_\_\_\_ Compound #:\_\_\_\_\_

(f)=RT Delta > 1/2 Window (m)=manual int.

HN006578.D HN1016NG.M Sat Nov 08 00:39:43 2014



# Quantitation Report


Signal #1 : Z:\HPCHEM1\HPLC\_N\DATA\HN102314\HN006578.D\VWD1A.CH Vial: 17  
 Signal #2 : Z:\HPCHEM1\HPLC\_N\DATA\HN102314\HN006578.D\VWD1A.CH  
 Acq On : 25-Oct-2014, 00:14 Operator: HNP  
 Sample : F4337-02MSD Inst : G1314A  
 Misc : Multiplr: 1.00  
 IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e  
 Quant Time: Oct 27 0:19 2014 Quant Results File: HN1016NG.RES

Instrument :  
 HPLC\_N  
 ClientSampleId :  
 YS19-SB21-1014MSD

Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN1016NG.M  
 Title :  
 Last Update : Fri Oct 17 04:15:53 2014  
 Response via : Multiple Level Calibration  
 DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul  
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

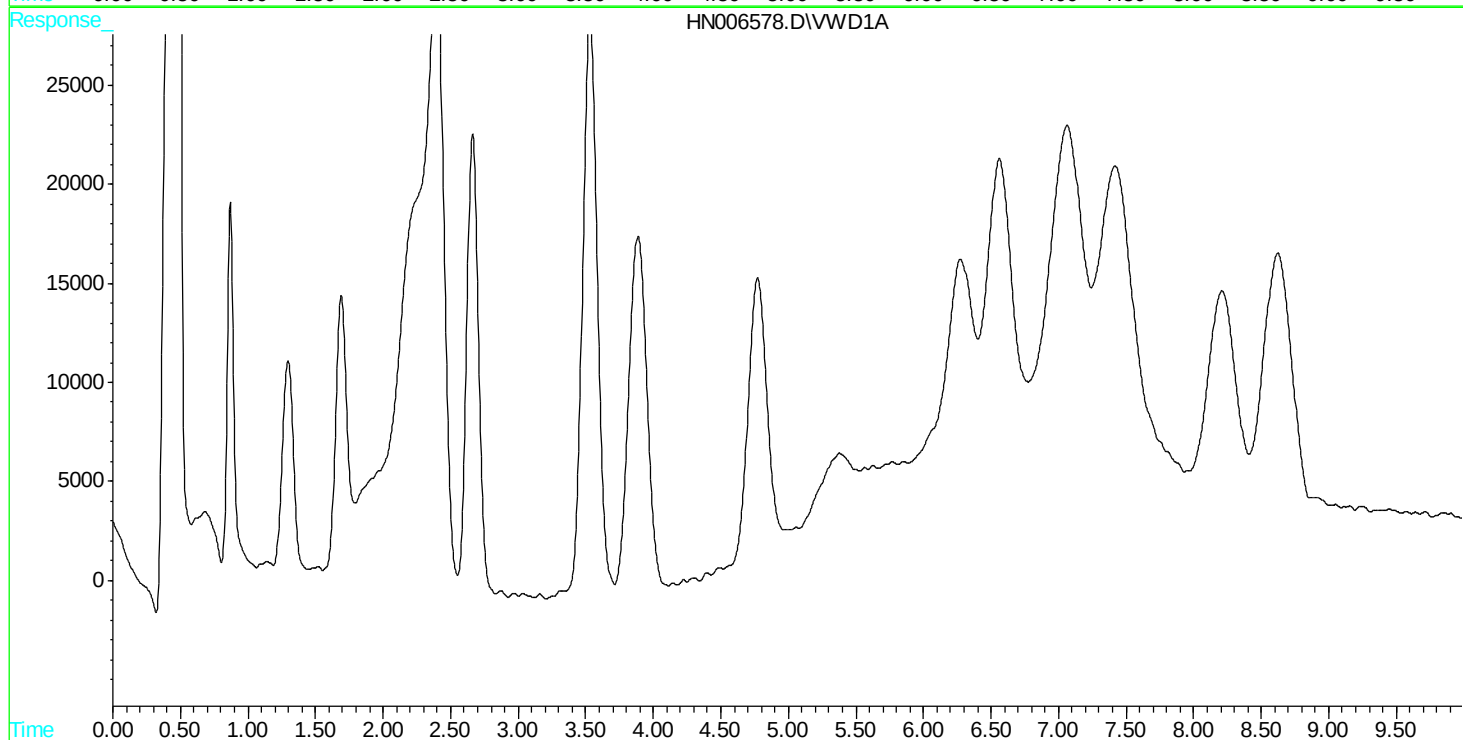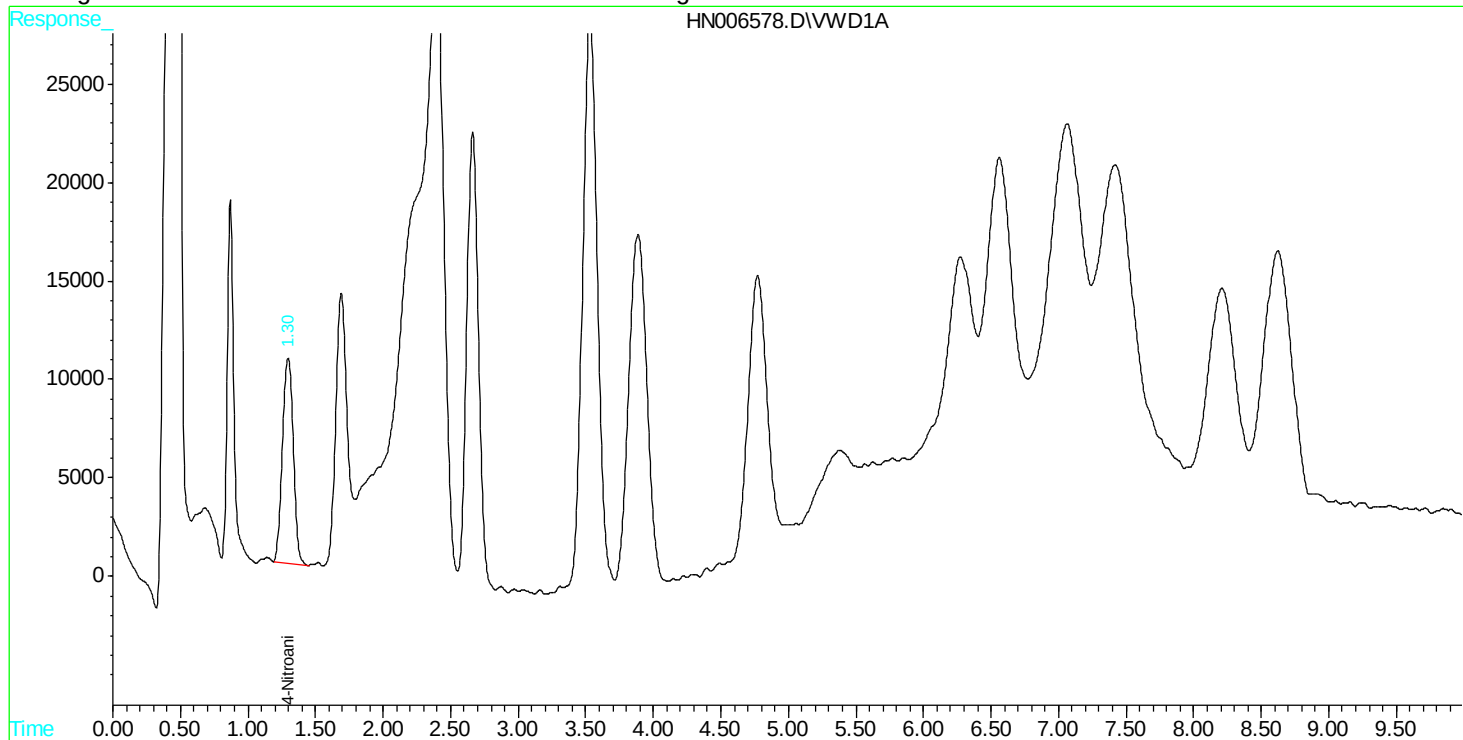

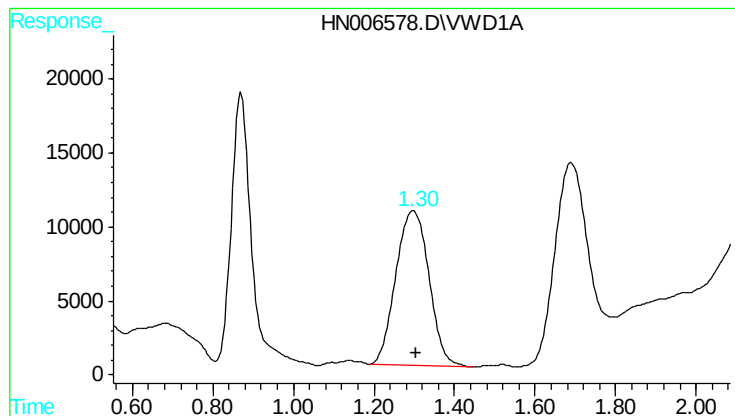

#1 4-Nitroaniline

R.T.: 1.298 min  
Delta R.T.: -0.007 min  
Response: 599539  
Conc: 0.15 ng/ul

Instrument :  
HPLC\_N  
ClientSampleId :  
YS19-SB21-1014MSD