

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN102314\HN006638.D\VWD1A.CH Vial: 91
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN102314\HN006638.D\VWD1A.CH
 Acq On : 25-Oct-2014, 12:15 Operator: HNP
 Sample : HSTDCCC005 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
 Quant Time: Oct 27 0:51 2014 Quant Results File: HN1016NG.RES

Instrument :
 HPLC_N
 LabSampleId :
 HSTDCCC005

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1016NG.M
 Title :
 Last Update : Fri Oct 17 04:15:53 2014
 Response via : Initial Calibration
 DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.30	18811951	4.736 ng/ul
Target Compounds			
2) T Nitroglycerin	6.04	38470865	5.023 ng/ul

 Analyst Signature: _____ Analyst Name: _____ Date: _____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #: _____

___Peak Integrated by software incorrectly.Compound #: _____

___OTHER: _____ Compound #: _____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN006638.D HN1016NG.M Sat Nov 08 00:57:18 2014



Quantitation Report


Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN102314\HN006638.D\VWD1A.CH Vial: 91
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN102314\HN006638.D\VWD1A.CH
 Acq On : 25-Oct-2014, 12:15 Operator: HNP
 Sample : HSTDCCC005 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
 Quant Time: Oct 27 0:51 2014 Quant Results File: HN1016NG.RES

Instrument :
 HPLC_N
 LabSampleId :
 HSTDCCC005

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1016NG.M
 Title :
 Last Update : Fri Oct 17 04:15:53 2014
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

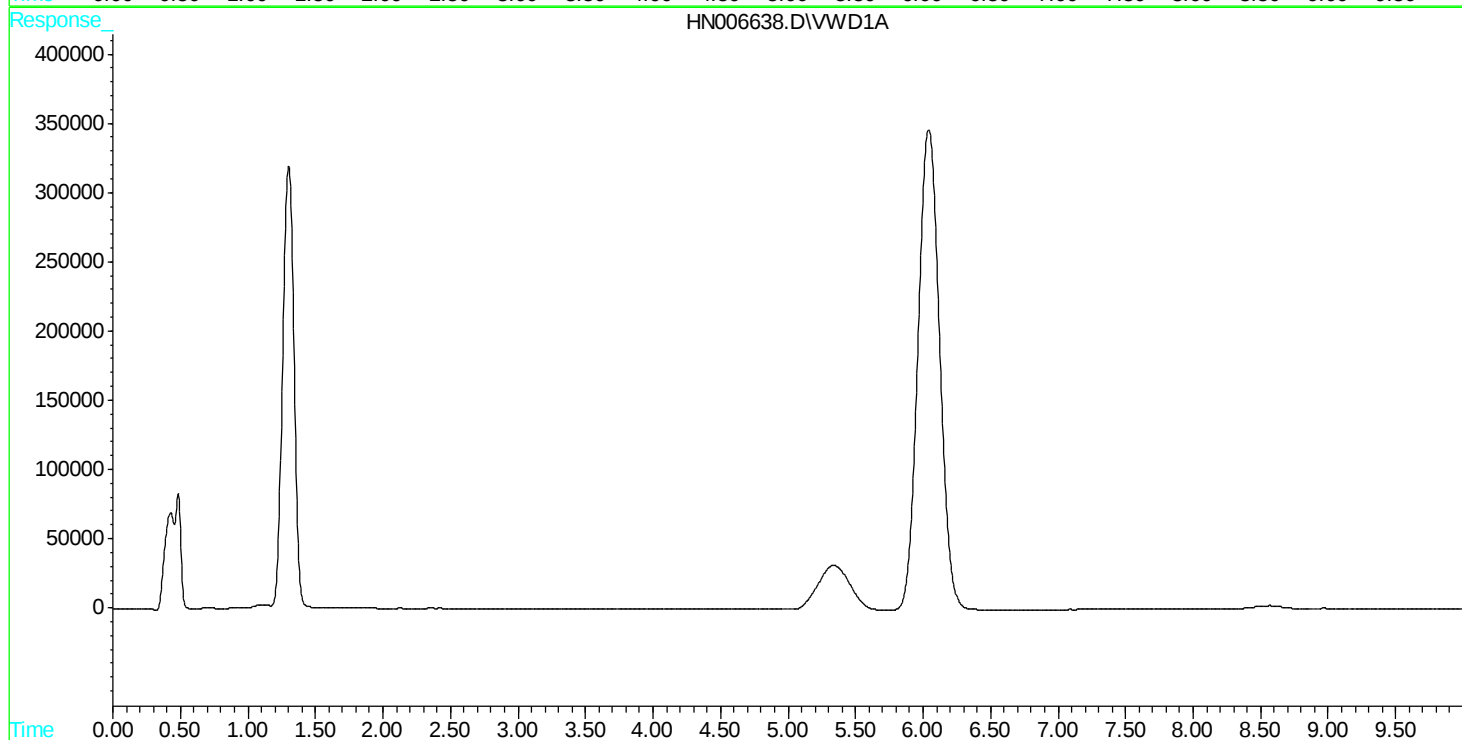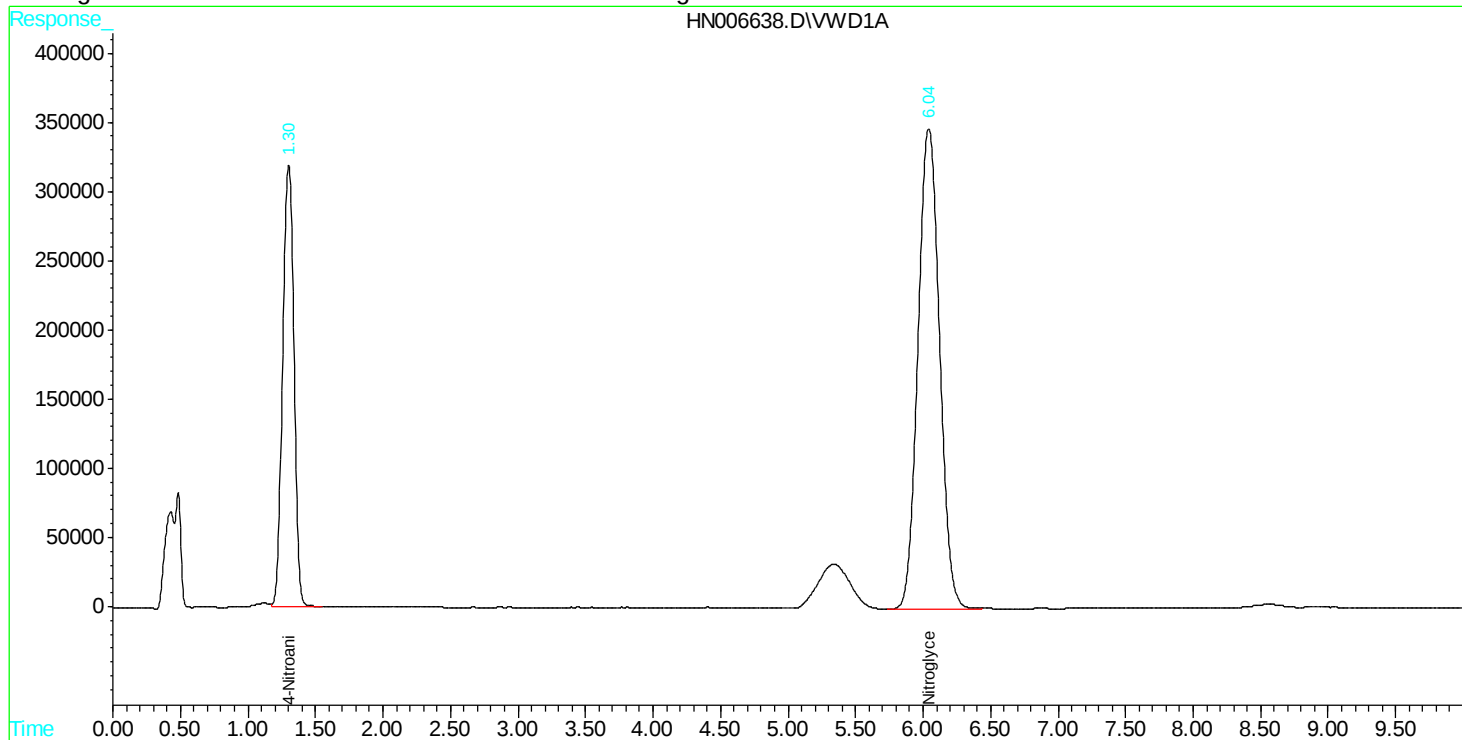


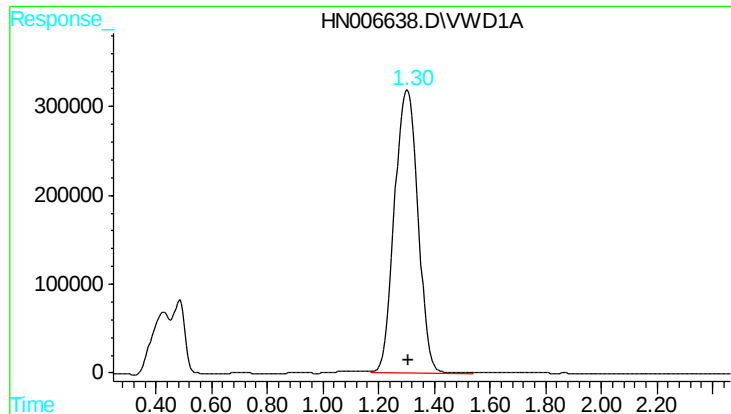

#1 4-Nitroaniline

R.T.: 1.303 min
Delta R.T.: -0.003 min
Response: 18811951
Conc: 4.74 ng/u1

Instrument :
HPLC_N
LabSampleId :
HSTDCCC005

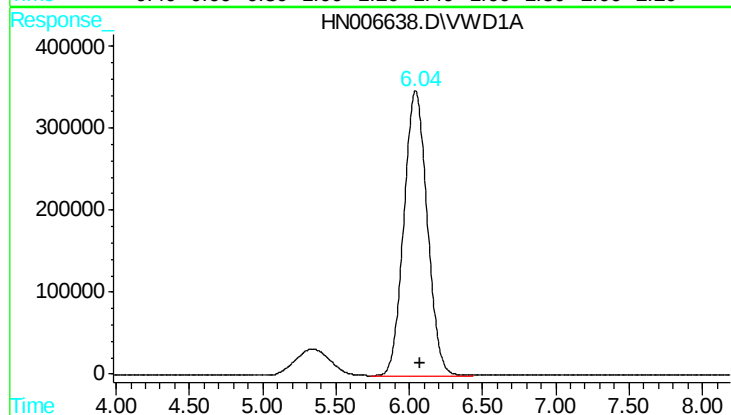

#2 Nitroglycerin

R.T.: 6.043 min
Delta R.T.: -0.031 min
Response: 38470865
Conc: 5.02 ng/u1