

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN102314\HN006650.D\VWD1A.CH Vial: 83
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN102314\HN006650.D\VWD1A.CH
 Acq On : 25-Oct-2014, 14:39 Operator: HNP
 Sample : 4368-10MSD Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
 Quant Time: Oct 28 0:22 2014 Quant Results File: HN1016NG.RES

Instrument :
 HPLC_N
 ClientSampleId :
 YS19-SB40-1014MSD

Manual Integrations
 APPROVED

ugo
 11/3/2014 11:53:37 AM

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1016NG.M
 Title :
 Last Update : Fri Oct 17 04:15:53 2014
 Response via : Initial Calibration
 DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.30	615454	0.155 ng/ul
Target Compounds			
2) T Nitroglycerin	6.03	978745	0.128 ng/ulm

 Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____ Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN006650.D HN1016NG.M Sat Nov 08 01:00:03 2014

Quantitation Report

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN102314\HN006650.D\VWD1A.CH Vial: 83
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN102314\HN006650.D\VWD1A.CH
 Acq On : 25-Oct-2014, 14:39 Operator: HNP
 Sample : 4368-10MSD Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
 Quant Time: Oct 28 0:22 2014 Quant Results File: HN1016NG.RES



Instrument :
 HPLC_N
 ClientSampleId :
 YS19-SB40-1014MSD


Manual Integrations
 APPROVED

ugo
 11/3/2014 11:53:37 AM

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1016NG.M
 Title :
 Last Update : Fri Oct 17 04:15:53 2014
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

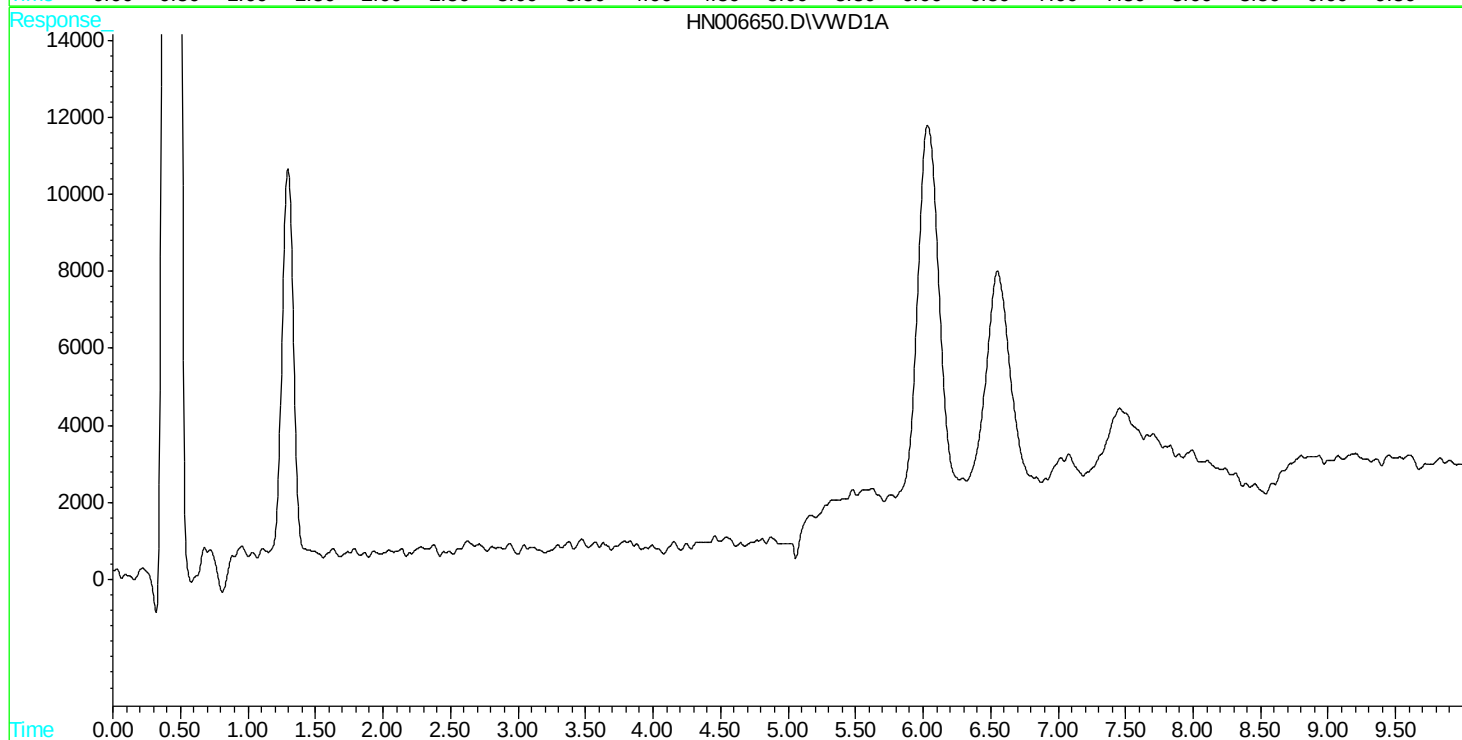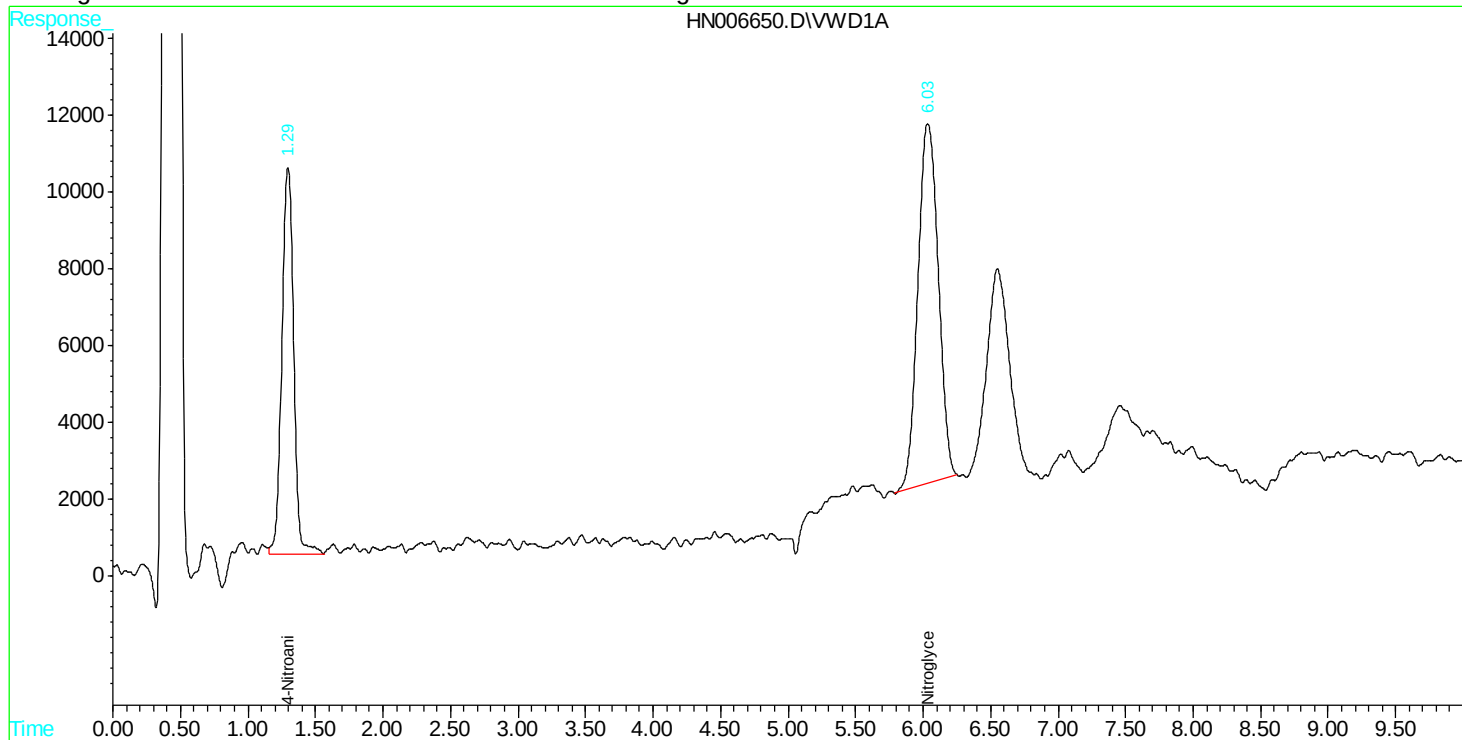

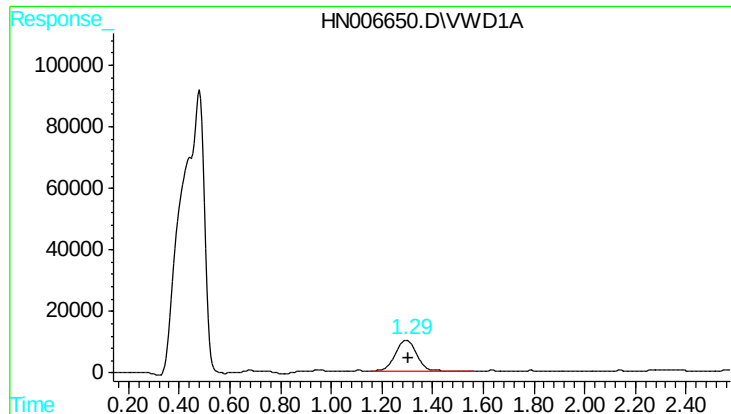


#1 4-Nitroaniline

R.T.: 1.297 min
Delta R.T.: -0.009 min
Response: 615454
Conc: 0.15 ng/ul

Instrument :
HPLC_N
ClientSampleId :
YS19-SB40-1014MSD

Manual Integrations
APPROVED

ugo
11/3/2014 11:53:37 AM

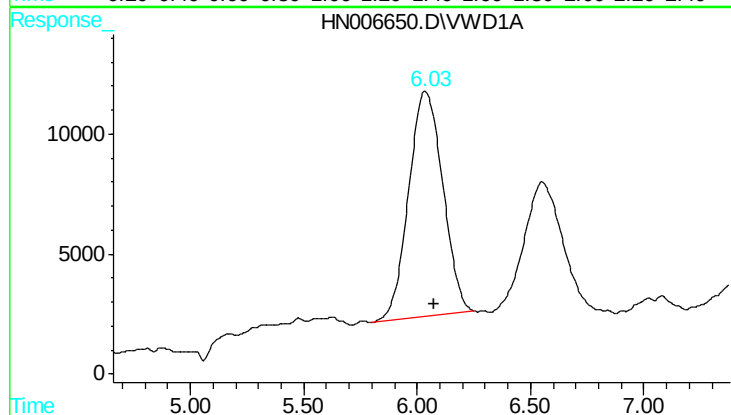

#2 Nitroglycerin

R.T.: 6.033 min
Delta R.T.: -0.042 min
Response: 978745
Conc: 0.13 ng/ul m