

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN102314\HN006652.D\VWD1A.CH Vial: 85
Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN102314\HN006652.D\VWD1A.CH
Acq On : 25-Oct-2014, 15:03 Operator: HNP
Sample : F4368-13MSD Inst : G1314A
Misc : Multiplr: 1.00
IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
Quant Time: Oct 28 0:23 2014 Quant Results File: HN1016NG.RES

Instrument :
HPLC_N
ClientSampleId :
YS19-SS39-1014MSD

Manual Integrations
APPROVED

ugo
11/3/2014 11:53:42 AM

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1016NG.M
Title :
Last Update : Fri Oct 17 04:15:53 2014
Response via : Initial Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.30	625307	0.157 ng/ul
Target Compounds			
2) T Nitroglycerin	6.05	1033810	0.135 ng/ulm

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____ Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN006652.D HN1016NG.M Sat Nov 08 01:00:31 2014

Quantitation Report

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN102314\HN006652.D\VWD1A.CH Vial: 85
Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN102314\HN006652.D\VWD1A.CH
Acq On : 25-Oct-2014, 15:03 Operator: HNP
Sample : F4368-13MSD Inst : G1314A
Misc : Multiplr: 1.00
IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
Quant Time: Oct 28 0:23 2014 Quant Results File: HN1016NG.RES



Instrument :
HPLC_N
ClientSampleId :
YS19-SS39-1014MSD


Manual Integrations
APPROVED

ugo
11/3/2014 11:53:42 AM

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1016NG.M
Title :
Last Update : Fri Oct 17 04:15:53 2014
Response via : Multiple Level Calibration
DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

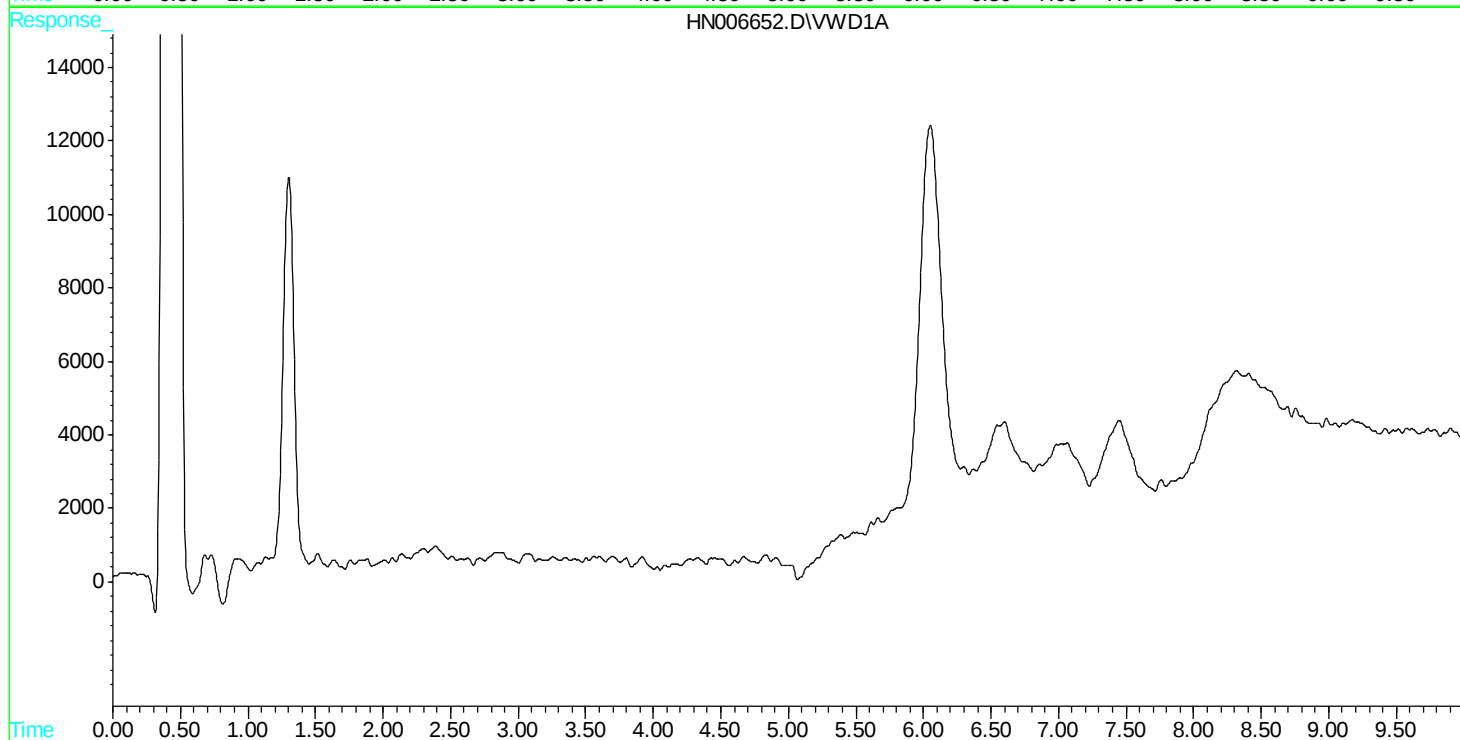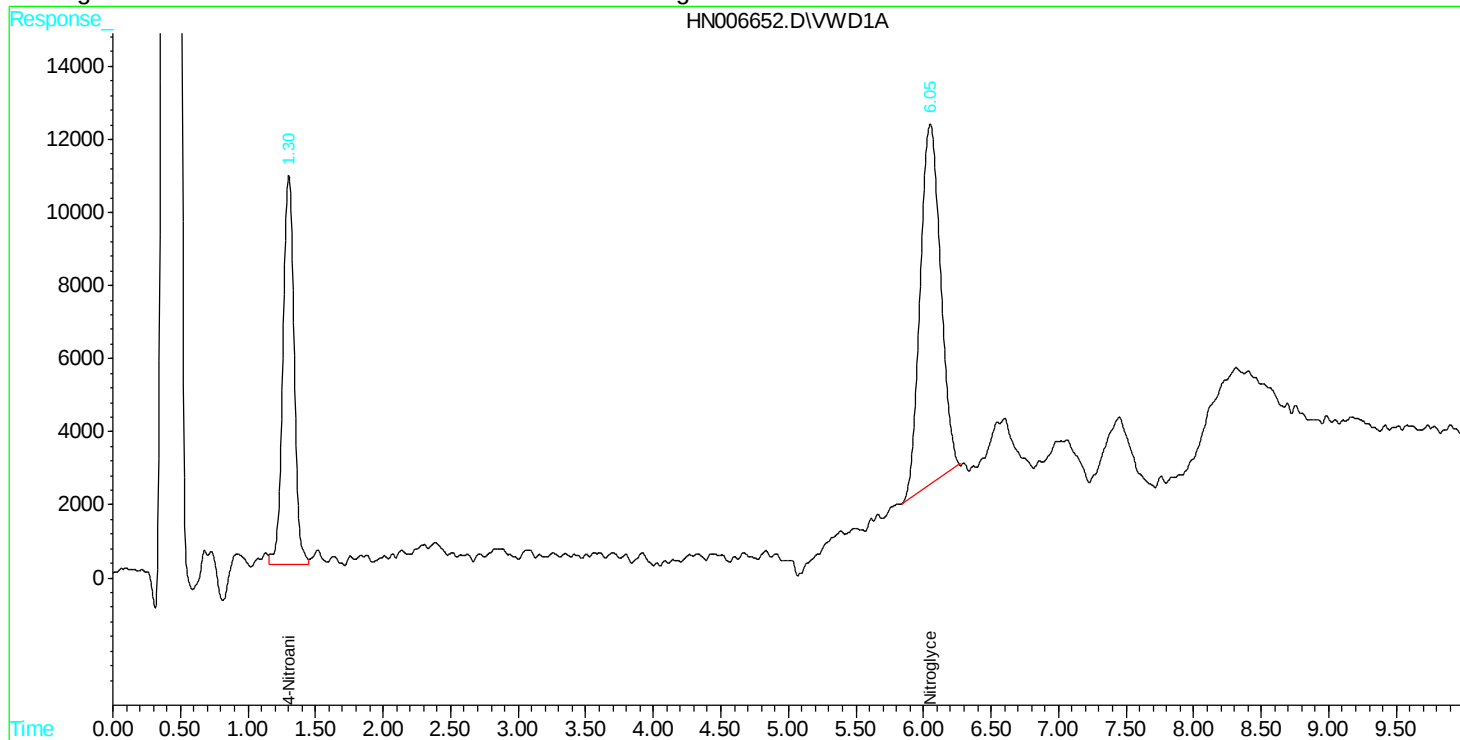

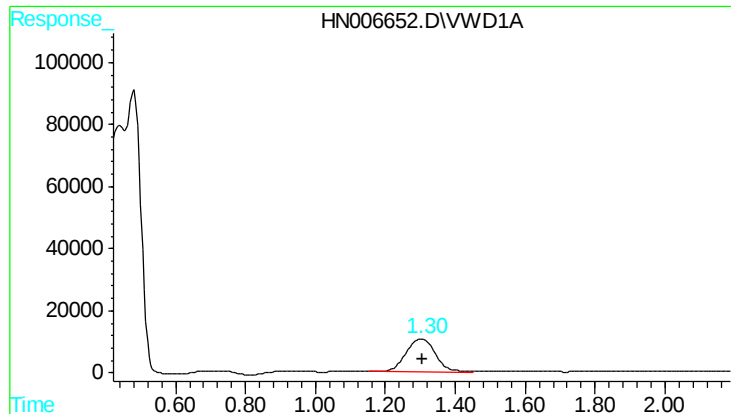


#1 4-Nitroaniline

R.T.: 1.304 min
Delta R.T.: -0.002 min
Response: 625307
Conc: 0.16 ng/u1

Instrument :
HPLC_N
ClientSampleId :
YS19-SS39-1014MSD

Manual Integrations
APPROVED

ugo
11/3/2014 11:53:42 AM

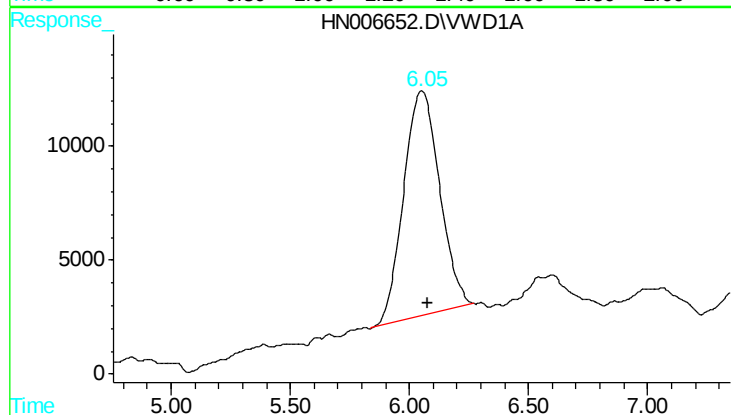

#2 Nitroglycerin

R.T.: 6.051 min
Delta R.T.: -0.023 min
Response: 1033810
Conc: 0.13 ng/u1 m