

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN102314\HN006654.D\VWD1A.CH Vial: 87
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN102314\HN006654.D\VWD1A.CH
 Acq On : 25-Oct-2014, 15:27 Operator: HNP
 Sample : LOQ-WATER Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
 Quant Time: Oct 28 0:36 2014 Quant Results File: HN1016NG.RES

Instrument :
 HPLC_N
 ClientSampleId :
 LOQ-WATER

Manual Integrations
 APPROVED

mohammad
 11/4/2014 10:08:08 AM

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1016NG.M
 Title :
 Last Update : Fri Oct 17 04:15:53 2014
 Response via : Initial Calibration
 DataAcq Meth : 8330ANG.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.30	1290955	0.325 ng/ul
Target Compounds			
2) T Nitroglycerin	6.05	829285	0.108 ng/ulm

 Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN006654.D HN1016NG.M Sat Nov 08 01:00:54 2014

Quantitation Report

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN102314\HN006654.D\VWD1A.CH Vial: 87
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN102314\HN006654.D\VWD1A.CH
 Acq On : 25-Oct-2014, 15:27 Operator: HNP
 Sample : LOQ-WATER Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: AUTOINT1.E IntFile Signal #2: autoint2.e
 Quant Time: Oct 28 0:36 2014 Quant Results File: HN1016NG.RES



Instrument :
 HPLC_N
 ClientSampleId :
 LOQ-WATER


Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN1016NG.M
 Title :
 Last Update : Fri Oct 17 04:15:53 2014
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330ANG.M

Manual Integrations
 APPROVED

mohammad
 11/4/2014 10:08:08 AM

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

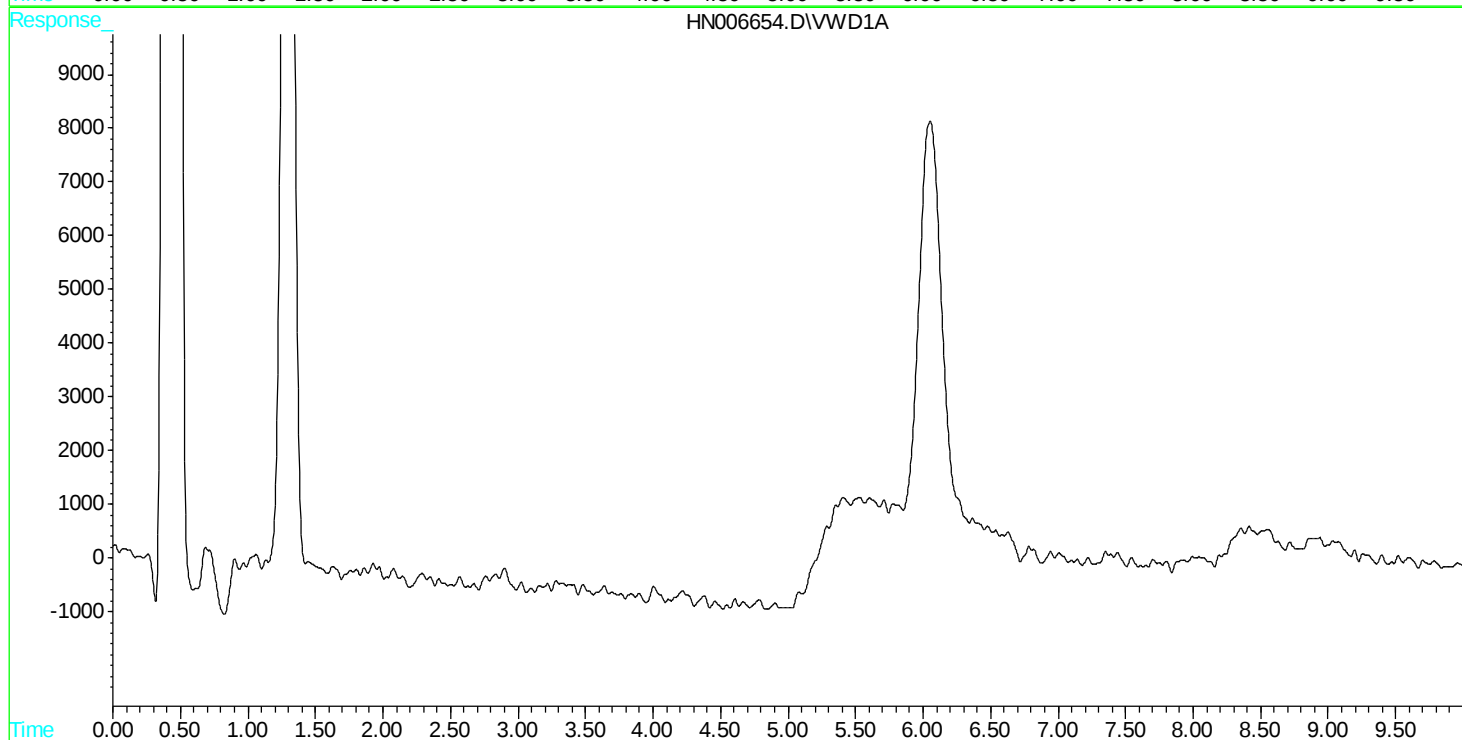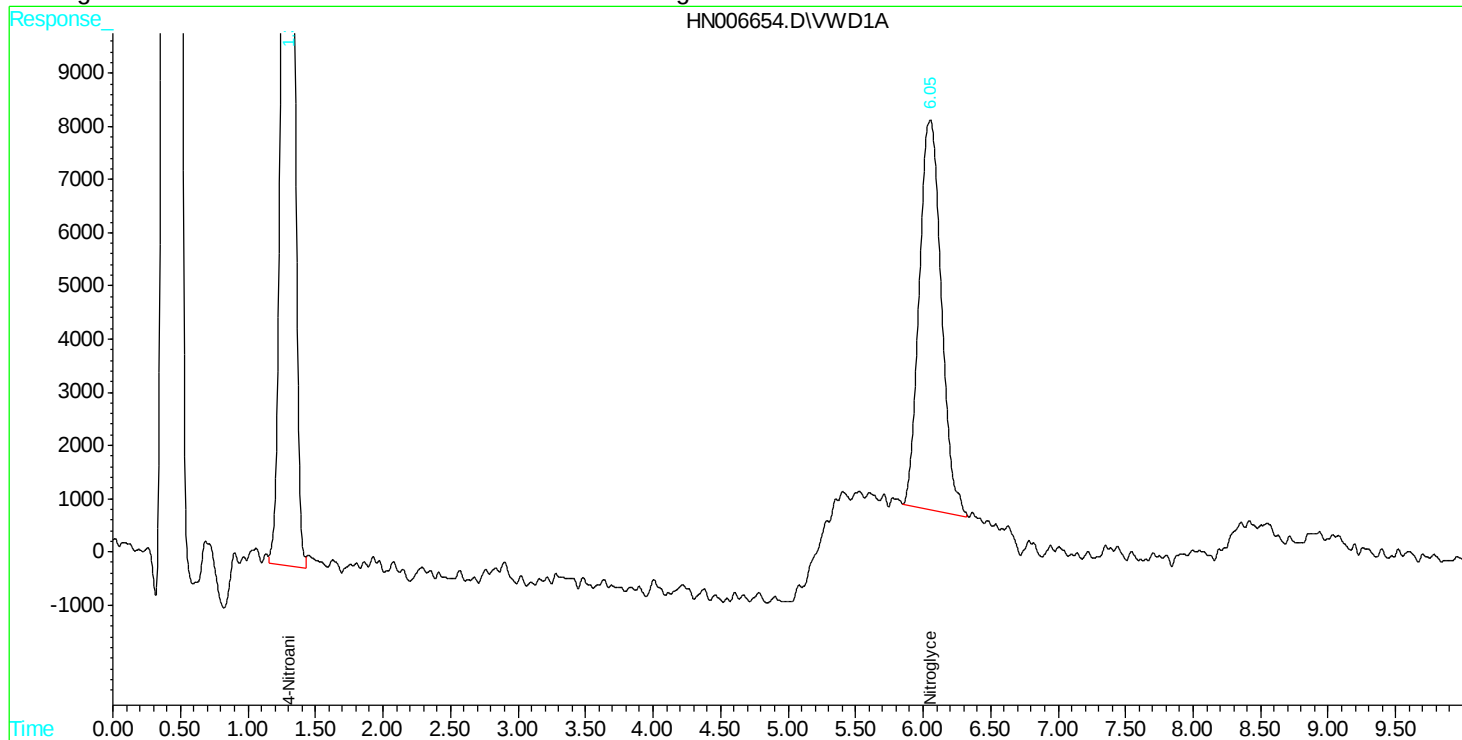

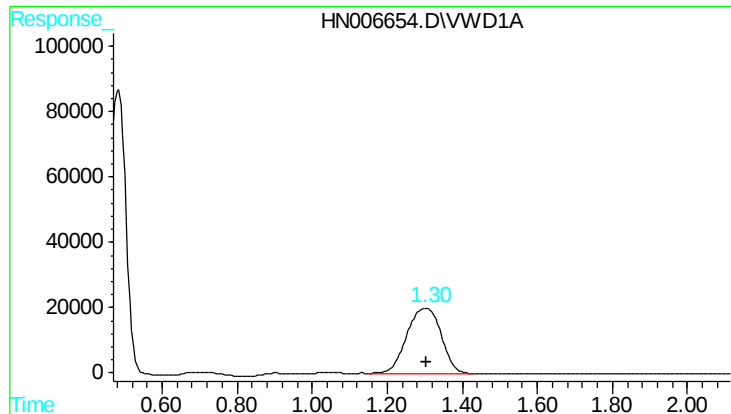


#1 4-Nitroaniline

R.T.: 1.304 min
Delta R.T.: -0.002 min
Response: 1290955
Conc: 0.33 ng/u1

Instrument :
HPLC_N
ClientSampleId :
LOQ-WATER

Manual Integrations
APPROVED

mohammad
11/4/2014 10:08:08 AM

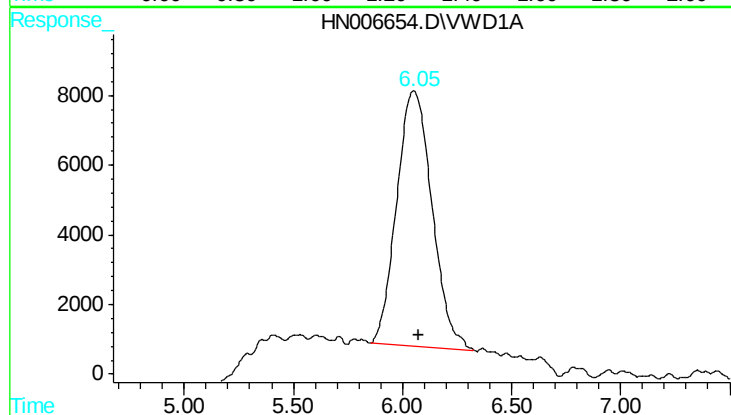

#2 Nitroglycerin

R.T.: 6.051 min
Delta R.T.: -0.023 min
Response: 829285
Conc: 0.11 ng/u1 m