

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN102714\
 Data File : HN006673.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 27-Oct-2014, 17:51
 Operator : TP
 Sample : F4351-05
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDCCC0500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 17:18:35 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
 Quant Title :
 QLast Update : Mon Mar 09 14:56:25 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 uL
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.316	998251	292.983 ug/L
Target Compounds			
2) T HMX	0.937	8445792	1873.522 ug/L
9) T 2,4,6-Trinitrotoluene	6.641	308978188	28168.206 ug/L
10) T 2-Amino-4,6-dinitroto...	7.144	99674880	8658.240 ug/L
11) T 4-Amino-2,6-dinitroto...	7.518	70017737	11436.274 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN102714\
Data File : HN006673.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 27-Oct-2014, 17:51
Operator : TP
Sample : F4351-05
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 17:18:35 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN100214.M
Quant Title :
QLast Update : Mon Mar 09 14:56:25 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

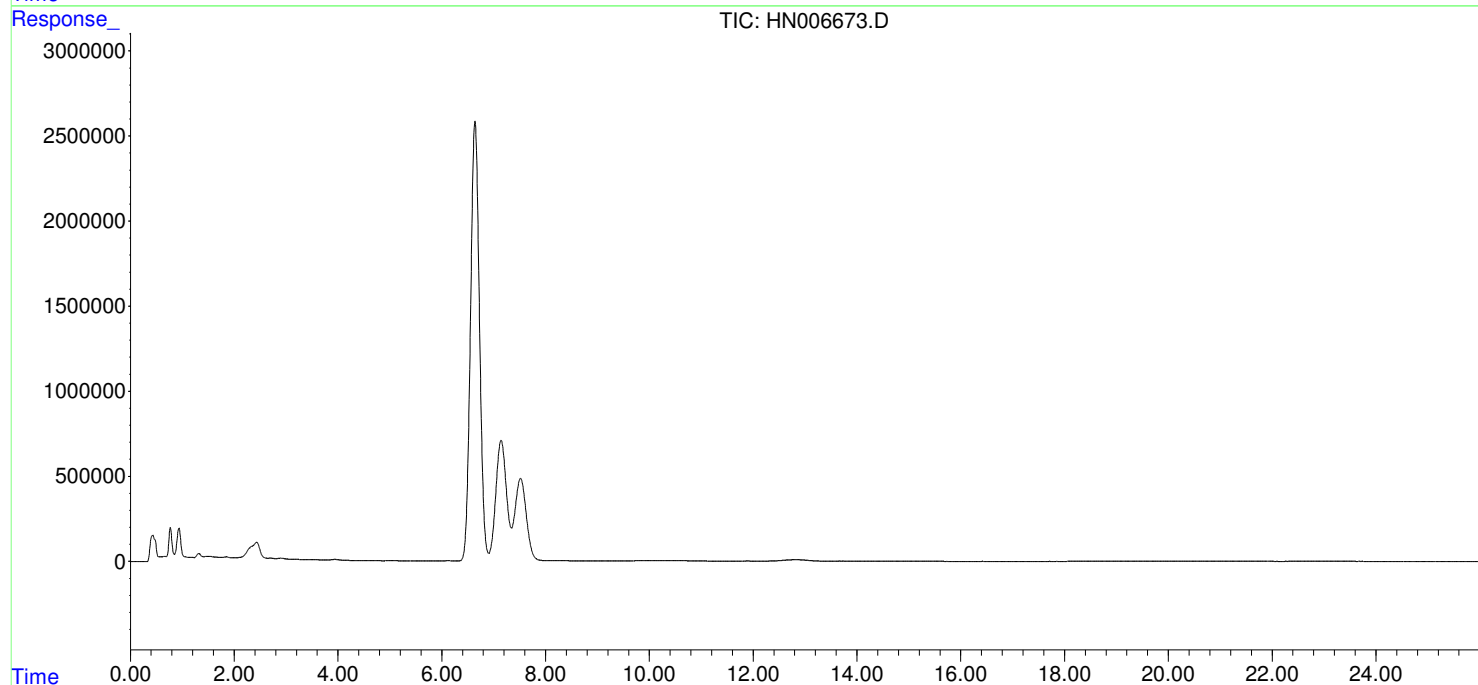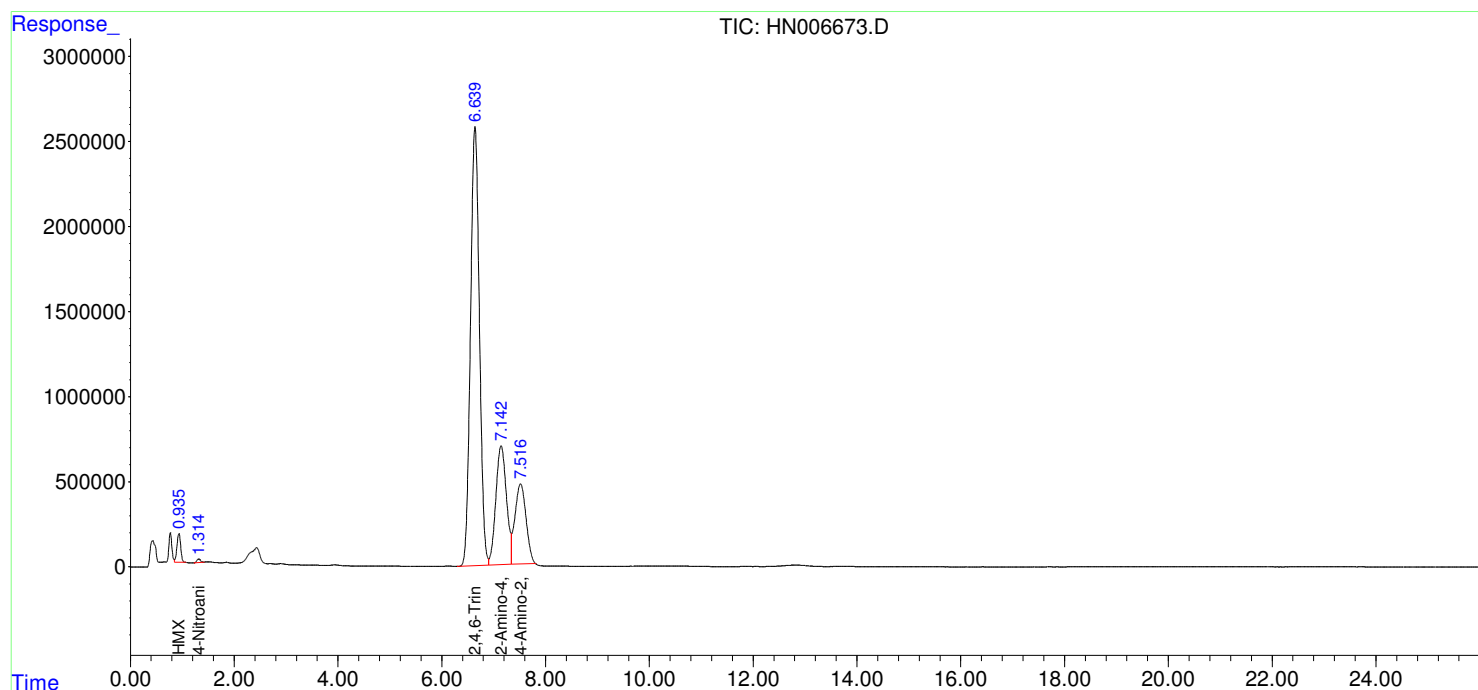


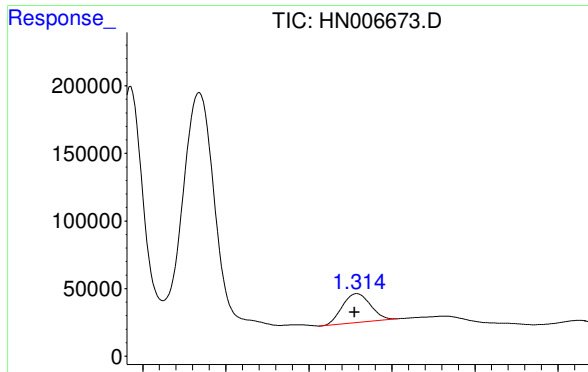

#1 4-Nitroaniline


R.T.: 1.316 min
Delta R.T.: 0.006 min
Response: 998251
Conc: 292.98 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

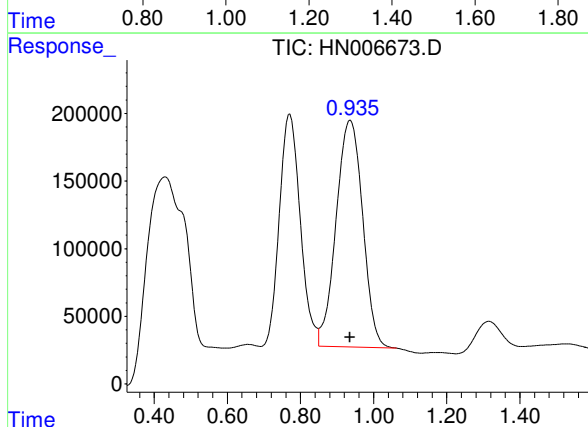


#2 HMX

R.T.: 0.937 min
Delta R.T.: 0.002 min
Response: 8445792
Conc: 1873.52 ug/L

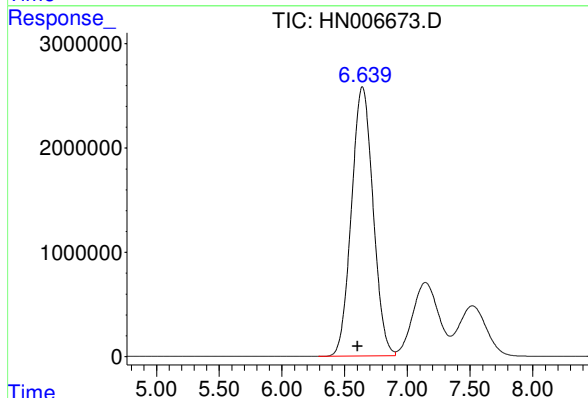


#9 2,4,6-Trinitrotoluene

R.T.: 6.641 min
Delta R.T.: 0.037 min
Response: 308978188
Conc: 28168.21 ug/L

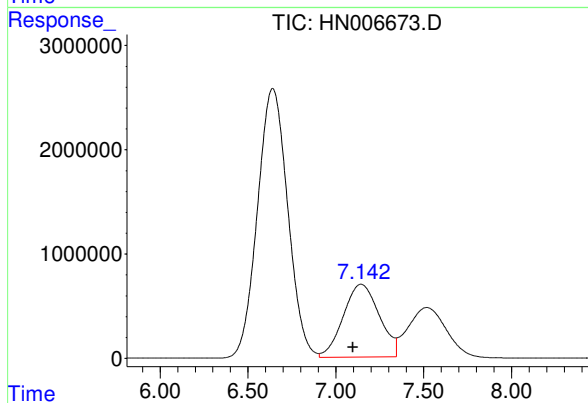

#10 2-Amino-4,6-dinitrotoluene

R.T.: 7.144 min
Delta R.T.: 0.048 min
Response: 99674880
Conc: 8658.24 ug/L

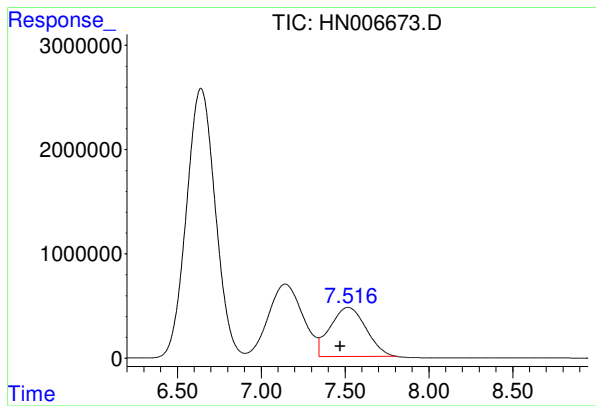

#11 4-Amino-2,6-dinitrotoluene

R.T.: 7.518 min
Delta R.T.: 0.048 min
Response: 70017737
Conc: 11436.27 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500