

Data Path : Z:\HPCHEM1\HPLC\_N\Data\HN102914\  
Data File : HN006837.D  
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
Acq On : 31-Oct-2014, 01:31  
Operator : TP  
Sample : F4372-07  
Misc :  
ALS Vial : 34 Sample Multiplier: 1

Instrument :  
HPLC\_N  
ClientSampleId :  
YS19-SD17-1014

Integration File signal 1: AUTOINT1.E  
Integration File signal 2: autoint2.e  
Quant Time: Mar 11 03:42:43 2015  
Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN1029NG.M  
Quant Title :  
QLast Update : Sat Mar 07 04:29:22 2015  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 u1  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

| Compound                    | R.T.  | Response | Conc Units  |
|-----------------------------|-------|----------|-------------|
| -----                       |       |          |             |
| System Monitoring Compounds |       |          |             |
| 1) S 4-Nitroaniline         | 1.303 | 599005   | 0.163 ng/u1 |
|                             |       |          |             |
| Target Compounds            |       |          |             |
| 2) T Nitroglycerin          | 6.052 | 2281     | 0.000 ng/u1 |
| -----                       |       |          |             |

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC\_N\Data\HN102914\  
Data File : HN006837.D  
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH  
Acq On : 31-Oct-2014, 01:31  
Operator : TP  
Sample : F4372-07  
Misc :  
ALS Vial : 34 Sample Multiplier: 1

Instrument :  
HPLC\_N  
ClientSampleId :  
YS19-SD17-1014

Integration File signal 1: AUTOINT1.E  
Integration File signal 2: autoint2.e  
Quant Time: Mar 11 03:42:43 2015  
Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN1029NG.M  
Quant Title :  
QLast Update : Sat Mar 07 04:29:22 2015  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 50 ul  
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

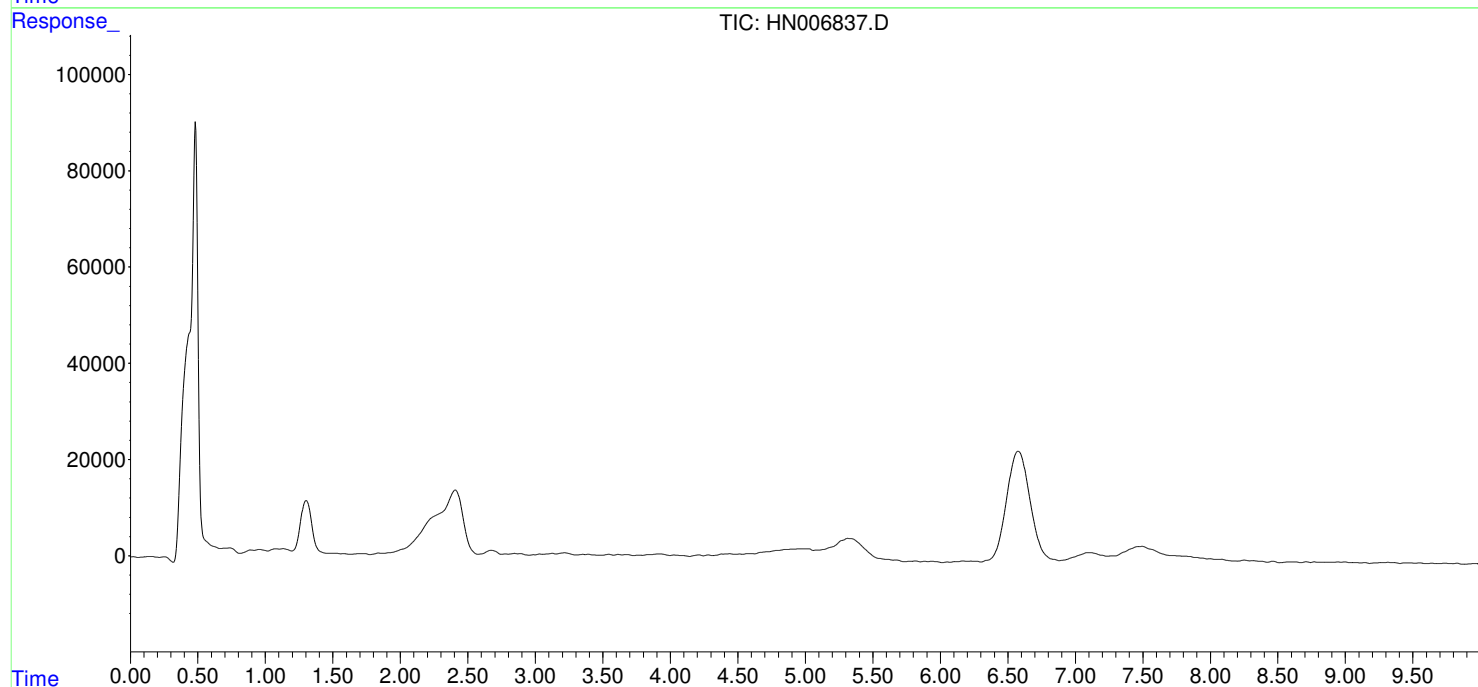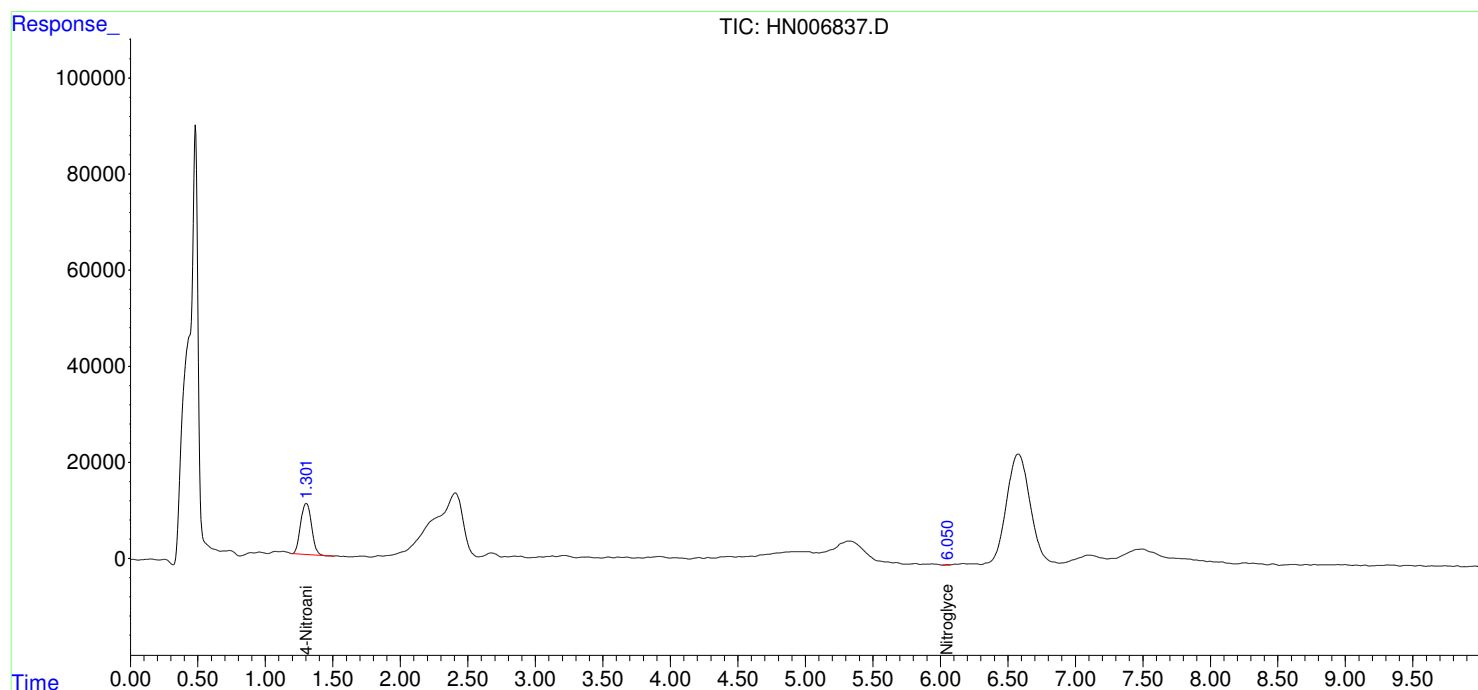


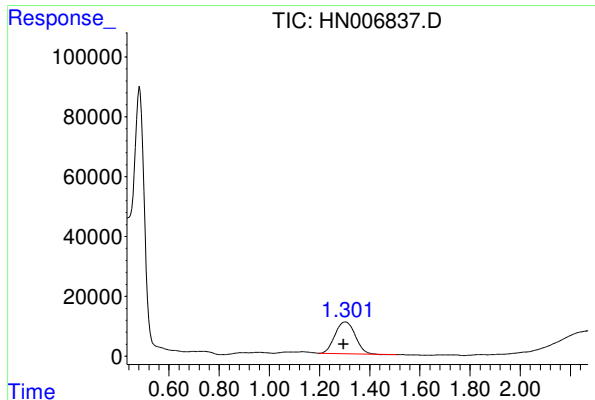

#1 4-Nitroaniline

R.T.: 1.303 min  
Delta R.T.: 0.007 min  
Response: 599005  
Conc: 0.16 ng/u1

Instrument :  
HPLC\_N  
ClientSampleId :  
YS19-SD17-1014

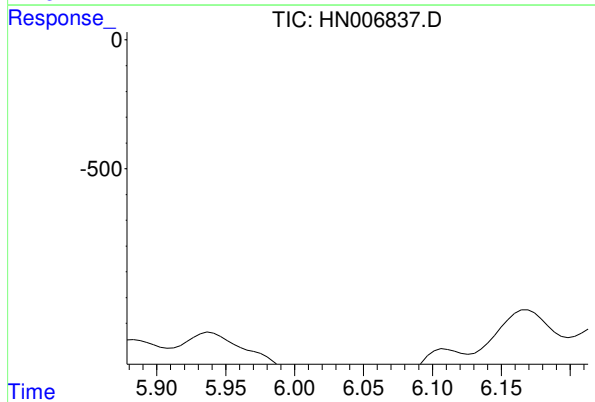

#2 Nitroglycerin

R.T.: 6.052 min  
Delta R.T.: 0.031 min  
Response: 2281  
Conc: 0.00 ng/u1