

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
Data File : HN006898.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 31-Oct-2014, 18:46
Operator : TP
Sample : HSTDICC1000
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 04:05:22 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Quant Title :
QLast Update : Sat Mar 07 03:03:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.292	2790551	799.517 ug/L
Target Compounds			
2) T HMX	0.866	3139569	745.295 ug/L
3) T RDX	1.679	4968879	982.535 ug/L
4) T 1,3,5-Trinitrobenzene	2.641f	10398237	1020.662 ug/L
8) T Tetryl	6.462	10188356	2223.874 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
Data File : HN006898.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 31-Oct-2014, 18:46
Operator : TP
Sample : HSTDICC1000
Misc :
ALS Vial : 73 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 04:05:22 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Quant Title :
QLast Update : Sat Mar 07 03:03:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

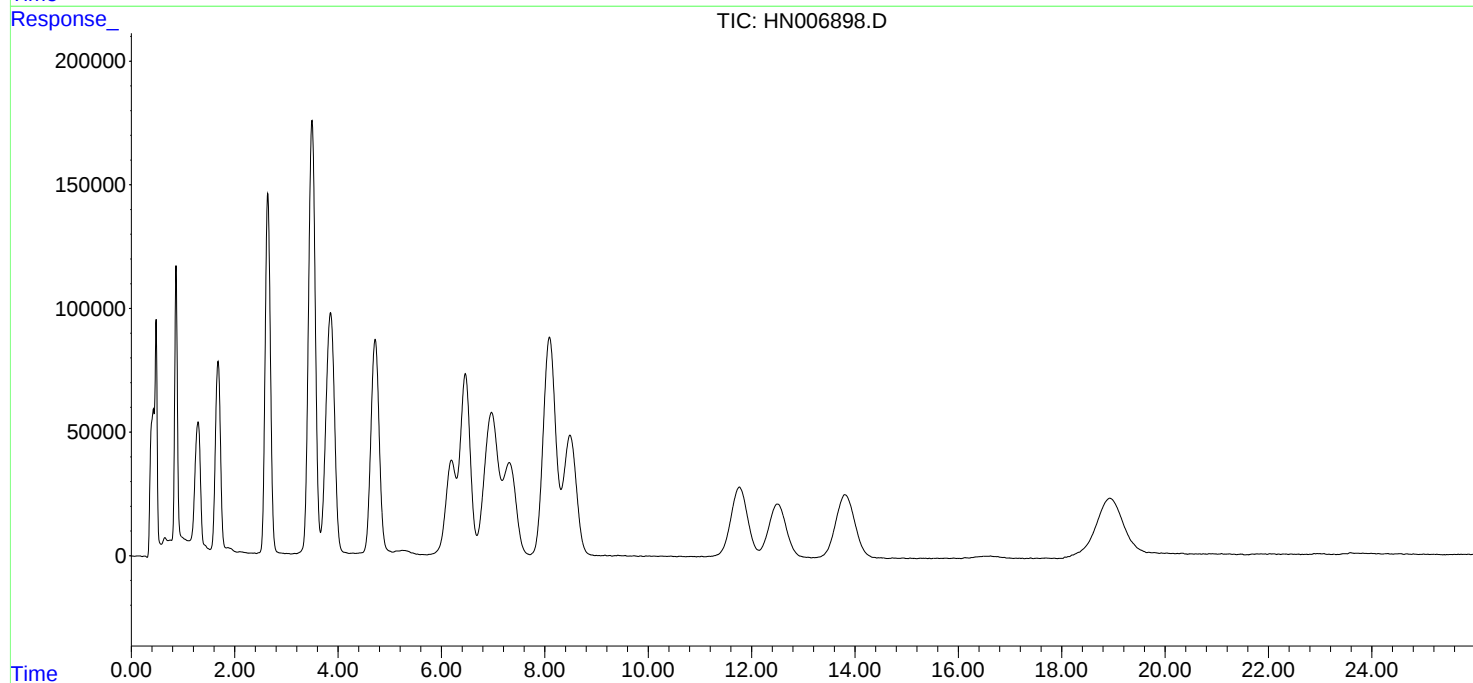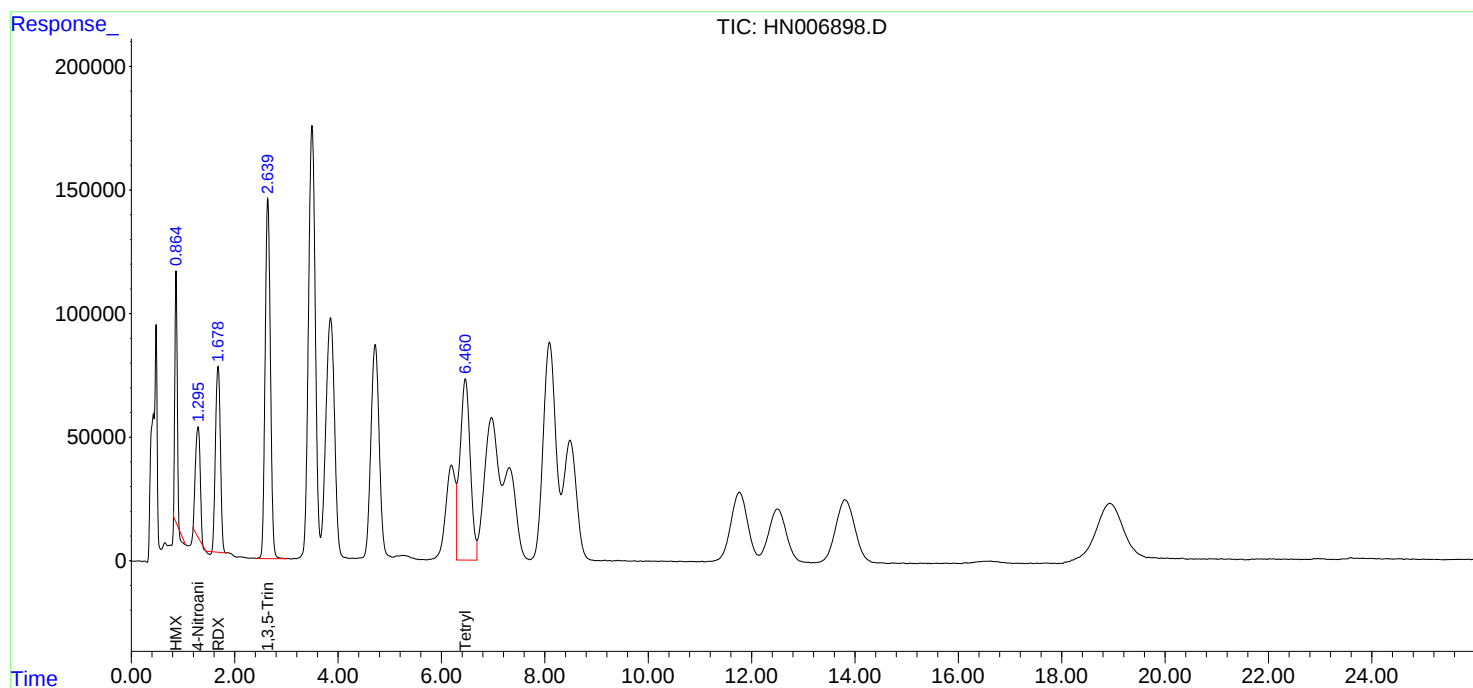


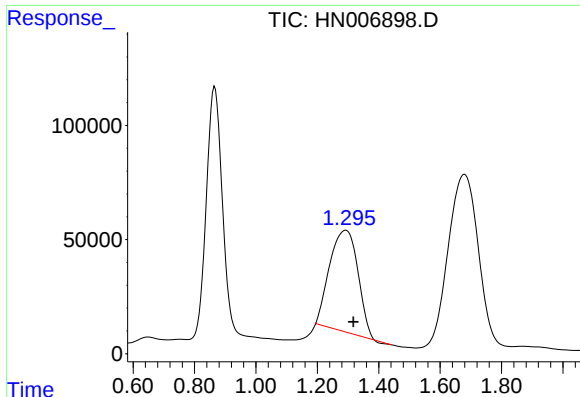

#1 4-Nitroaniline


R.T.: 1.292 min
Delta R.T.: -0.025 min
Response: 2790551
Conc: 799.52 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDICC1000

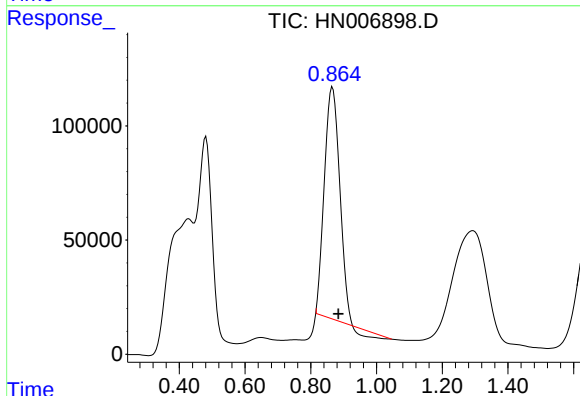


#2 HMX

R.T.: 0.866 min
Delta R.T.: -0.019 min
Response: 3139569
Conc: 745.30 ug/L

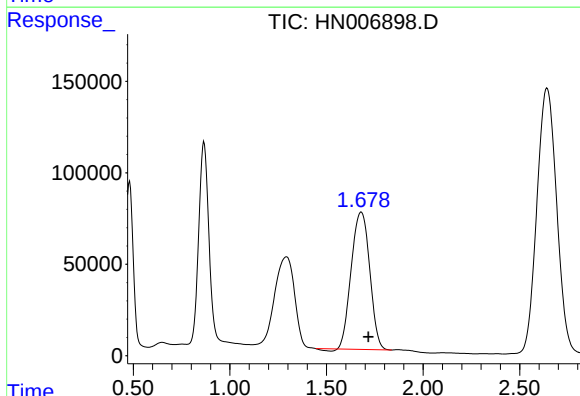


#3 RDX

R.T.: 1.679 min
Delta R.T.: -0.038 min
Response: 4968879
Conc: 982.54 ug/L

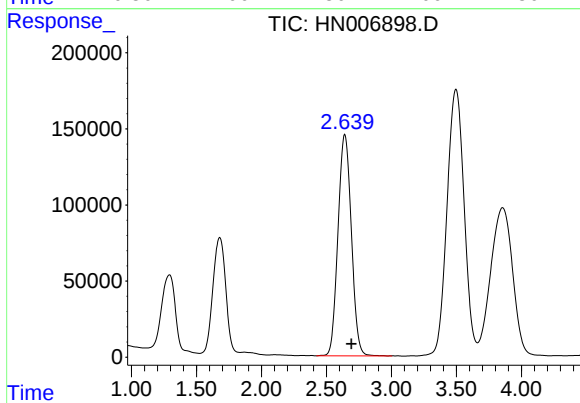

#4 1,3,5-Trinitrobenzene

R.T.: 2.641 min
Delta R.T.: -0.051 min
Response: 10398237
Conc: 1020.66 ug/L

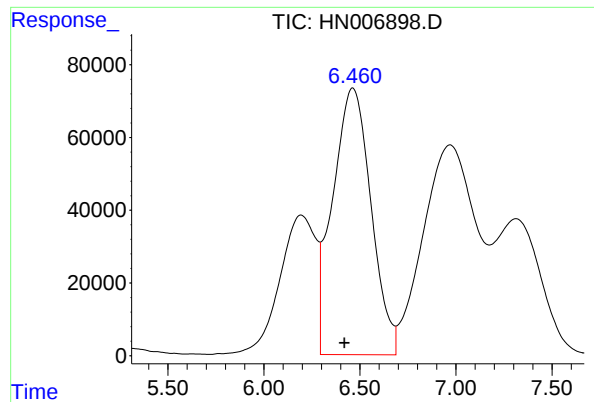

#8 Tetryl

R.T.: 6.462 min

Delta R.T.: 0.043 min

Response: 10188356

Conc: 2223.87 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDICC1000