

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
Data File : HN006899.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 31-Oct-2014, 19:14
Operator : TP
Sample : HSTDICCC0500
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDICCC0500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 04:05:28 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Quant Title :
QLast Update : Sat Mar 07 03:03:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.296	1402601	401.858 ug/L
Target Compounds			
2) T HMX	0.868	1740079	413.073 ug/L
3) T RDX	1.678	2512202	496.757 ug/L
4) T 1,3,5-Trinitrobenzene	2.648	5271161	517.403 ug/L
5) T 1,3-Dinitrobenzene	3.508f	8080656	506.528 ng/ml

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
Data File : HN006899.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 31-Oct-2014, 19:14
Operator : TP
Sample : HSTDICCC0500
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDICCC0500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 04:05:28 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Quant Title :
QLast Update : Sat Mar 07 03:03:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

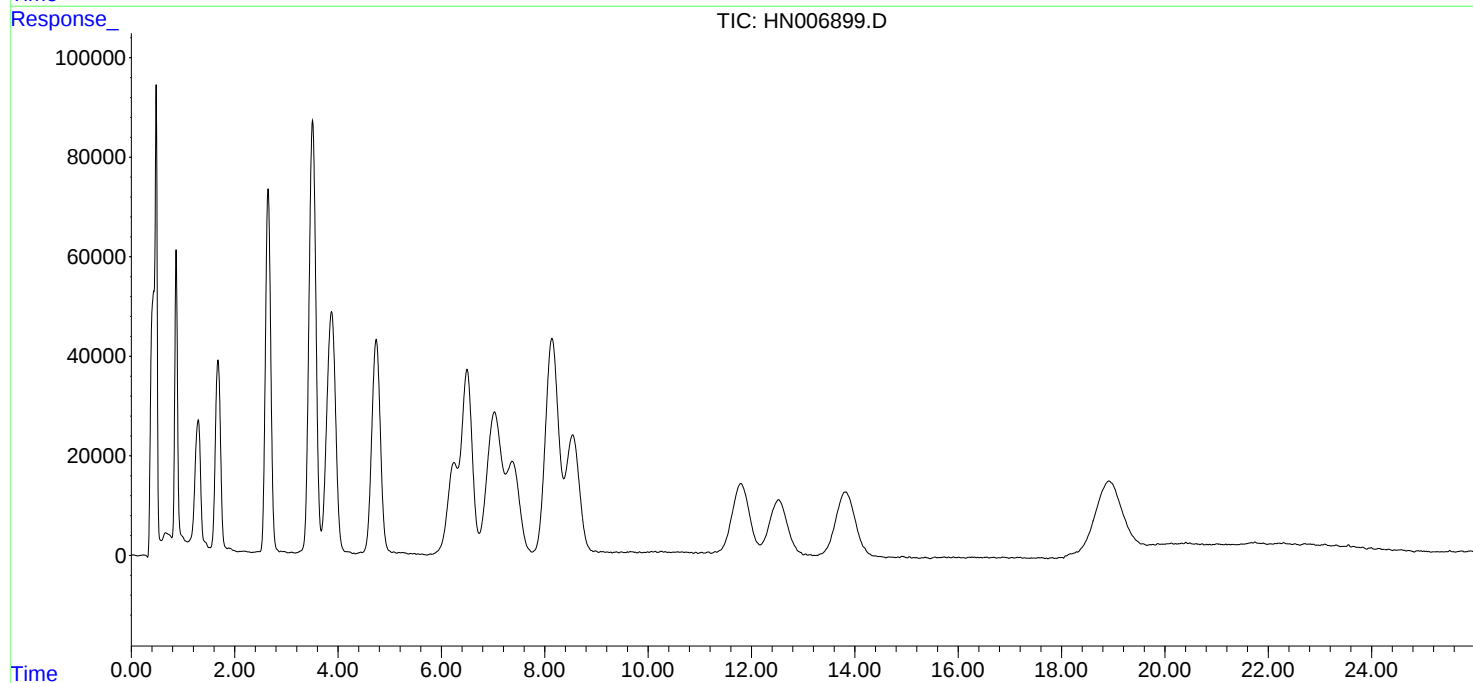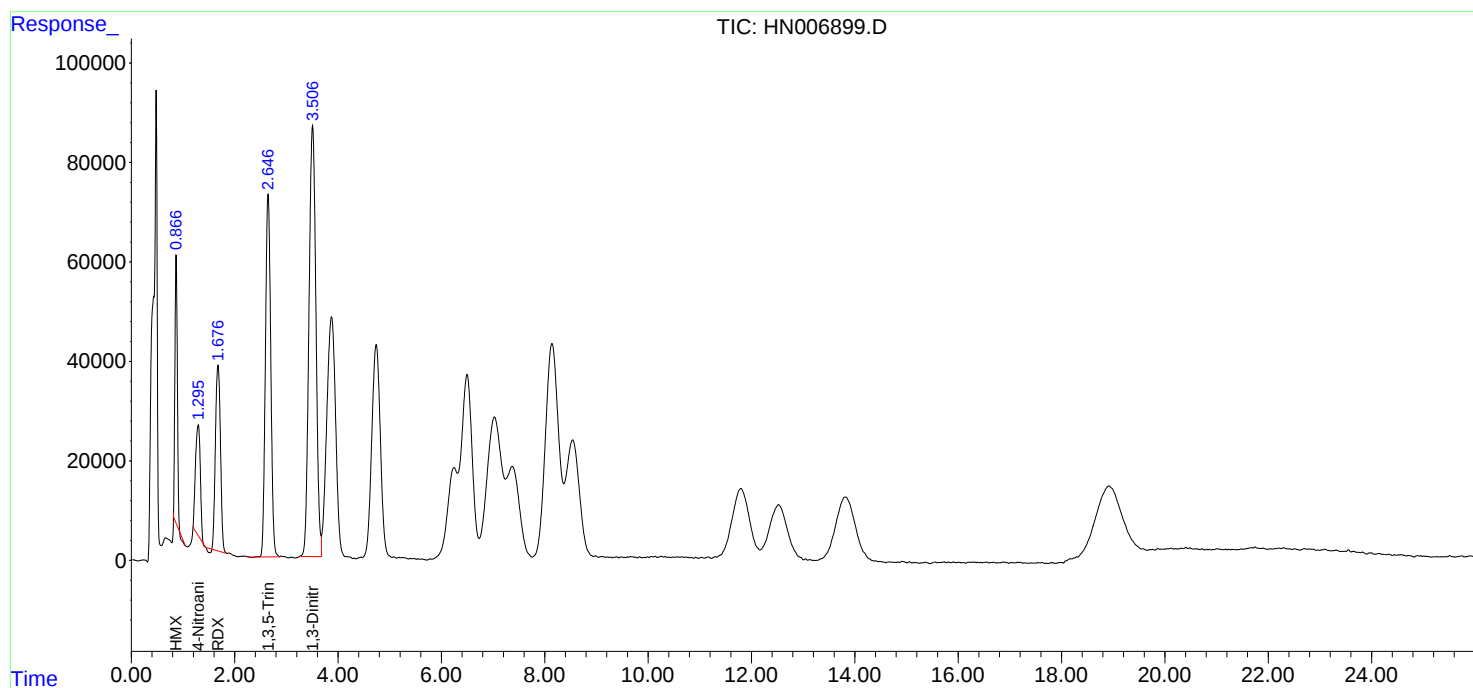


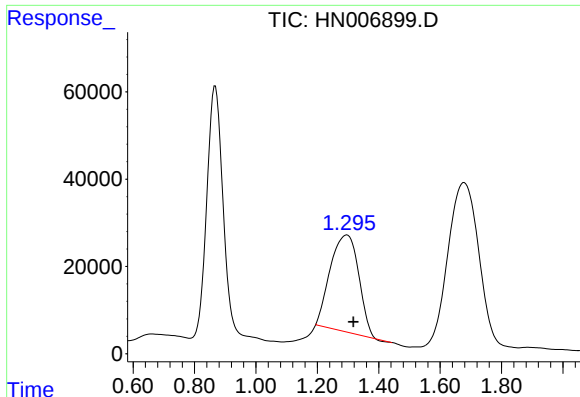

#1 4-Nitroaniline


R.T.: 1.296 min
Delta R.T.: -0.021 min
Response: 1402601
Conc: 401.86 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDICCC0500

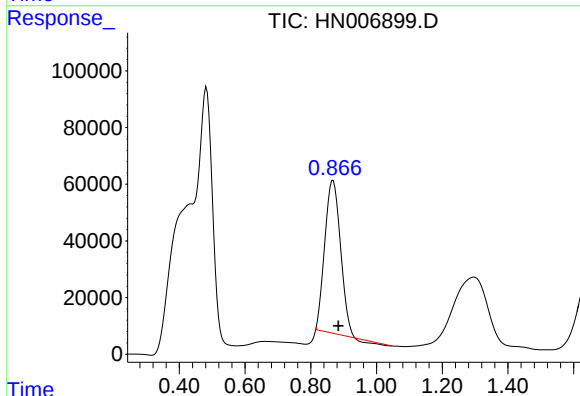


#2 HMX

R.T.: 0.868 min
Delta R.T.: -0.017 min
Response: 1740079
Conc: 413.07 ug/L

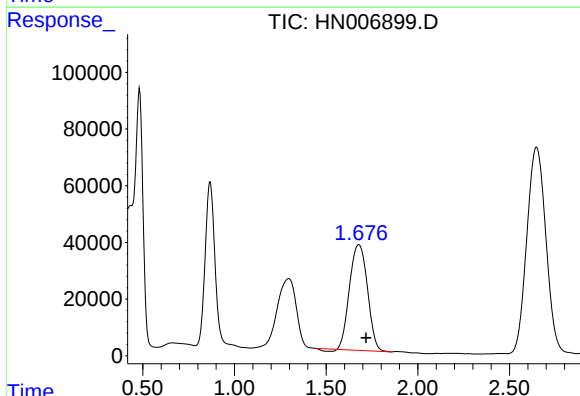


#3 RDX

R.T.: 1.678 min
Delta R.T.: -0.039 min
Response: 2512202
Conc: 496.76 ug/L

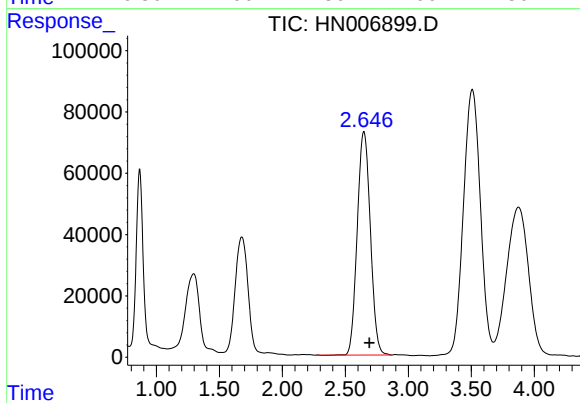

#4 1,3,5-Trinitrobenzene

R.T.: 2.648 min
Delta R.T.: -0.045 min
Response: 5271161
Conc: 517.40 ug/L

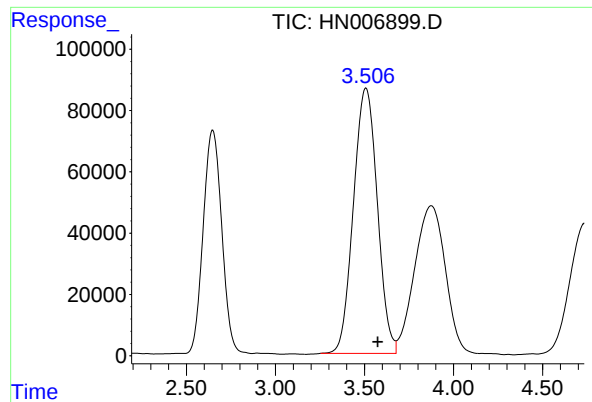

#5 1,3-Dinitrobenzene

R.T.: 3.508 min

Delta R.T.: -0.067 min

Response: 8080656

Conc: 506.53 ng/ml

Instrument :
HPLC_N
ClientSampleId :
HSTDICCC0500