

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
 Data File : HN006900.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 31-Oct-2014, 19:42
 Operator : TP
 Sample : HSTDICC0100
 Misc :
 ALS Vial : 75 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDICC0100

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 04:05:34 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
 Quant Title :
 QLast Update : Sat Mar 07 03:03:02 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.292	348104	99.735 ug/L
Target Compounds			
2) T HMX	0.869	462169	109.713 ug/L
3) T RDX	1.683	571445	112.996 ug/L
4) T 1,3,5-Trinitrobenzene	2.649	1184399	116.257 ug/L
5) T 1,3-Dinitrobenzene	3.509f	1793779	112.441 ng/ml

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
Data File : HN006900.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 31-Oct-2014, 19:42
Operator : TP
Sample : HSTDICC0100
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDICC0100

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 04:05:34 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Quant Title :
QLast Update : Sat Mar 07 03:03:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

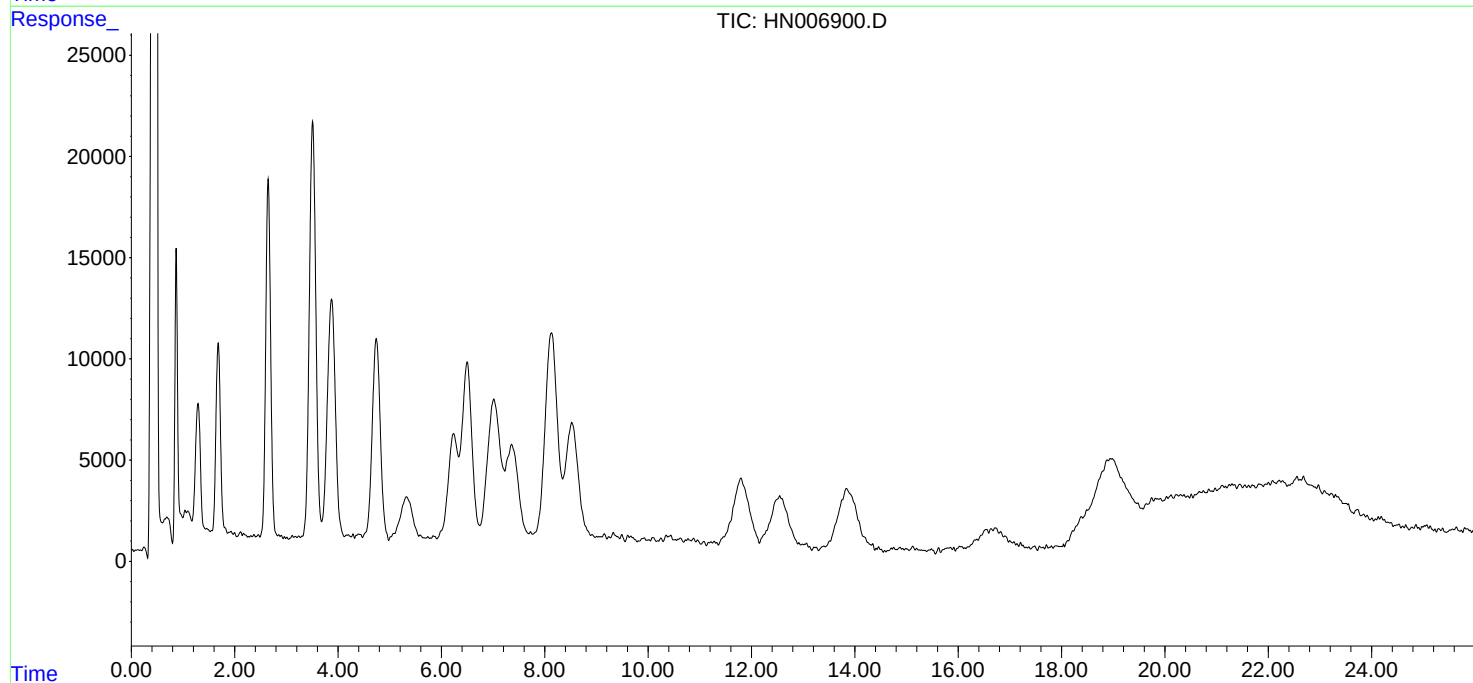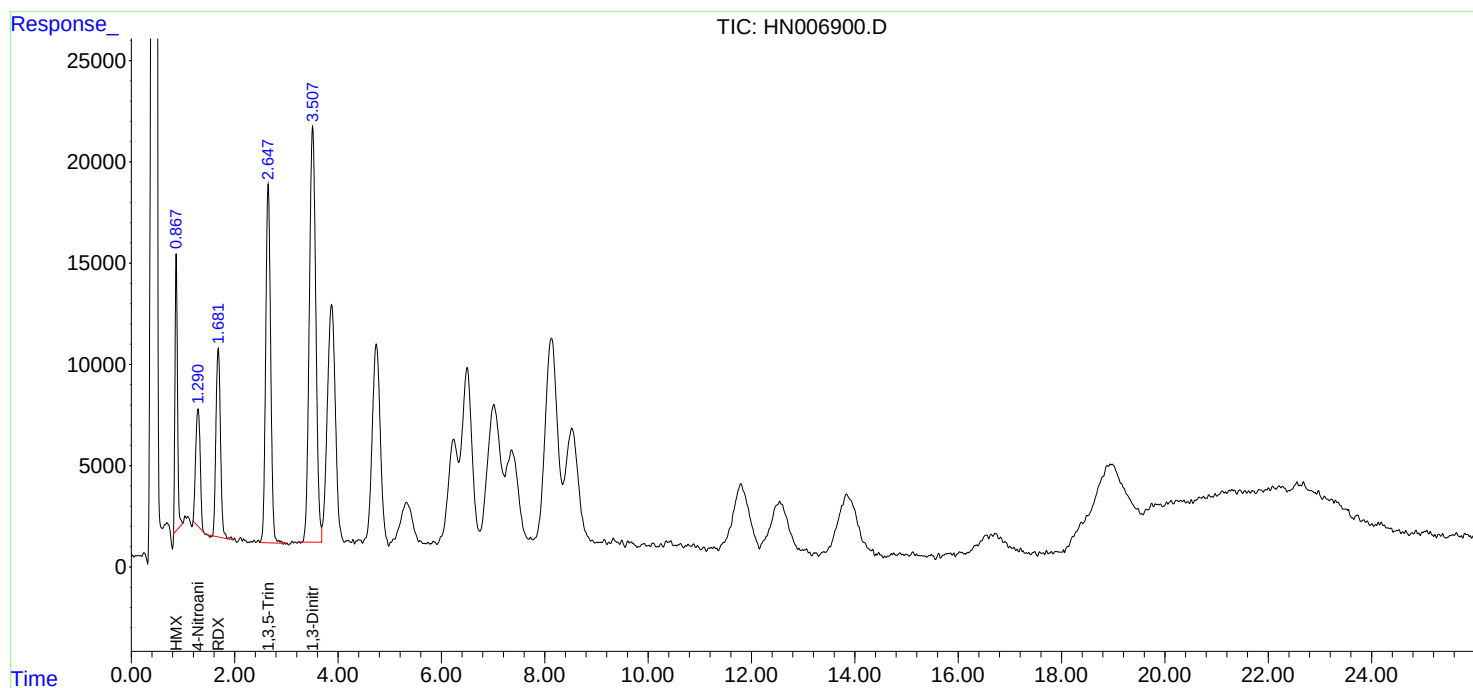


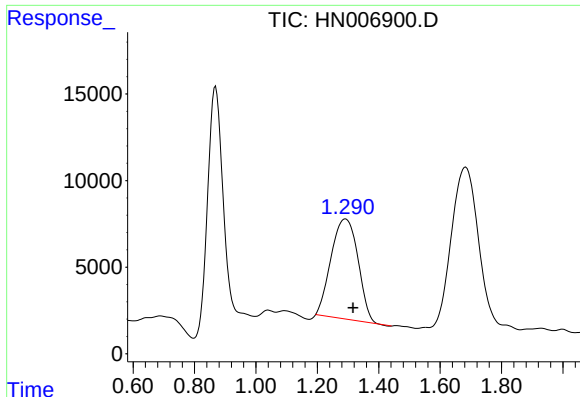

#1 4-Nitroaniline


R.T.: 1.292 min
Delta R.T.: -0.025 min
Response: 348104
Conc: 99.73 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDICC0100

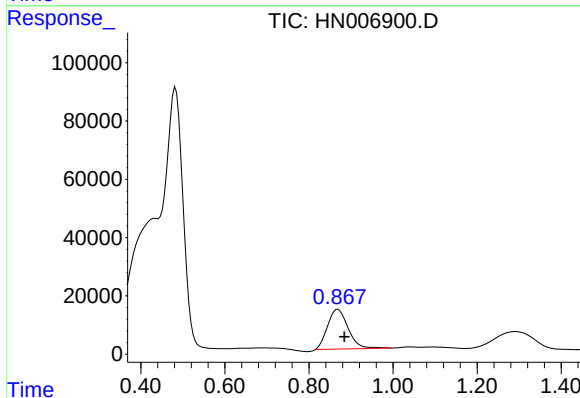


#2 HMX

R.T.: 0.869 min
Delta R.T.: -0.016 min
Response: 462169
Conc: 109.71 ug/L

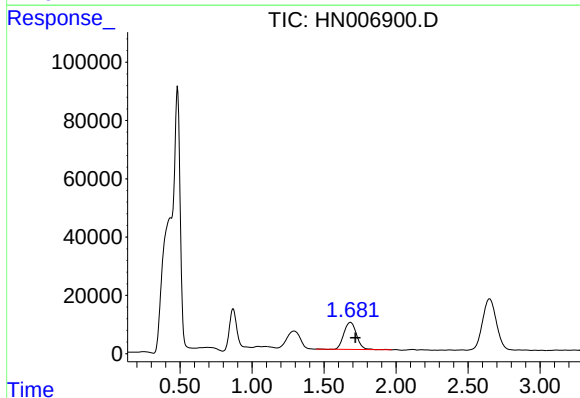


#3 RDX

R.T.: 1.683 min
Delta R.T.: -0.034 min
Response: 571445
Conc: 113.00 ug/L

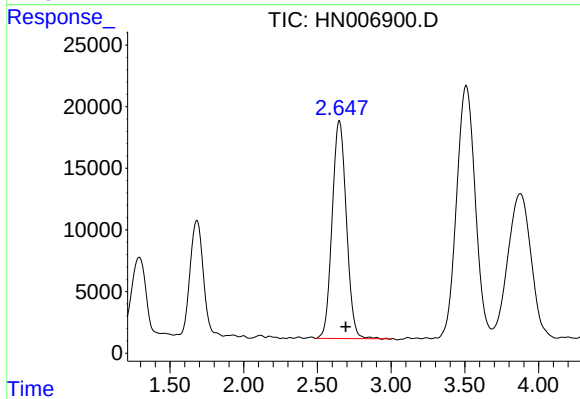

#4 1,3,5-Trinitrobenzene

R.T.: 2.649 min
Delta R.T.: -0.044 min
Response: 1184399
Conc: 116.26 ug/L

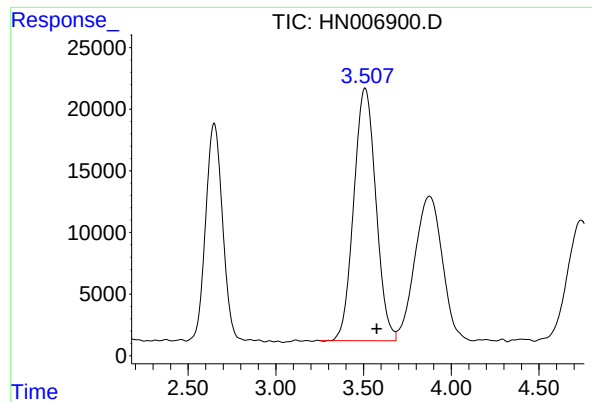

#5 1,3-Dinitrobenzene

R.T.: 3.509 min

Delta R.T.: -0.066 min

Response: 1793779

Conc: 112.44 ng/ml

Instrument :
HPLC_N
ClientSampleId :
HSTDICC0100