

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
Data File : HN006910.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 01-Nov-2014, 00:22
Operator : TP
Sample : F4372-03MSD
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
YS19-SD01-1014MSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 04:06:38 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Quant Title :
QLast Update : Sat Mar 07 03:03:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.294	529730	151.772 ug/L
Target Compounds			
2) T HMX	0.871	533847	126.729 ug/L
3) T RDX	1.686	577172	114.129 ug/L
4) T 1,3,5-Trinitrobenzene	2.650	765505	75.140 ug/L
5) T 1,3-Dinitrobenzene	3.509f	1524495	95.561 ng/ml

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
Data File : HN006910.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 01-Nov-2014, 00:22
Operator : TP
Sample : F4372-03MSD
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
YS19-SD01-1014MSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 04:06:38 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Quant Title :
QLast Update : Sat Mar 07 03:03:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

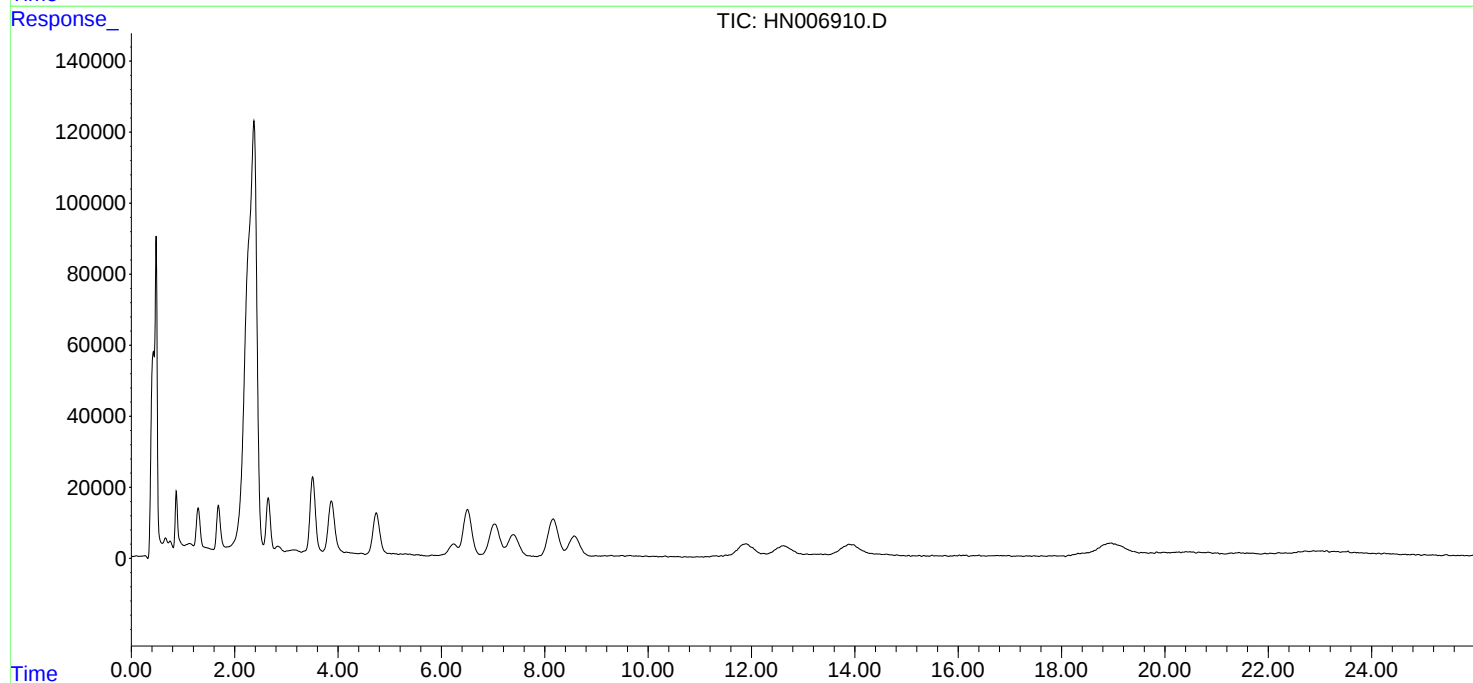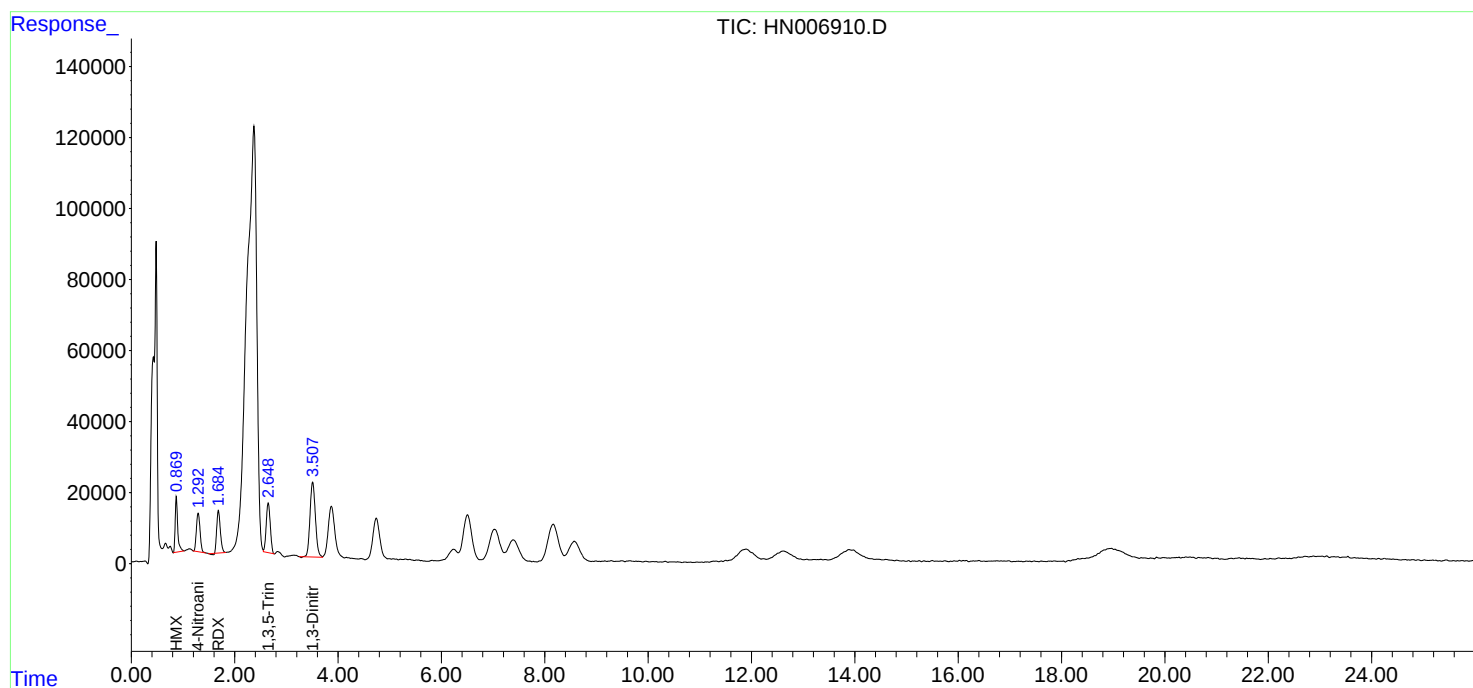


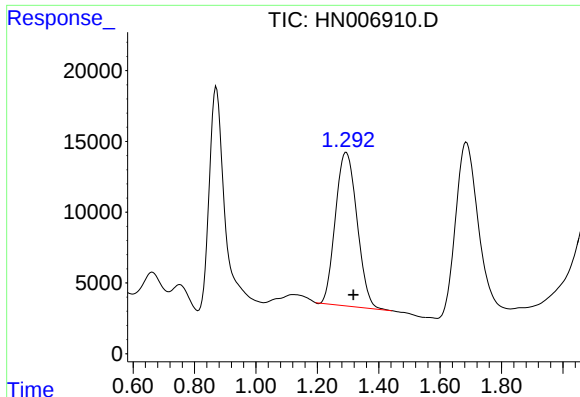

#1 4-Nitroaniline


R.T.: 1.294 min
Delta R.T.: -0.023 min
Response: 529730
Conc: 151.77 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-SD01-1014MSD

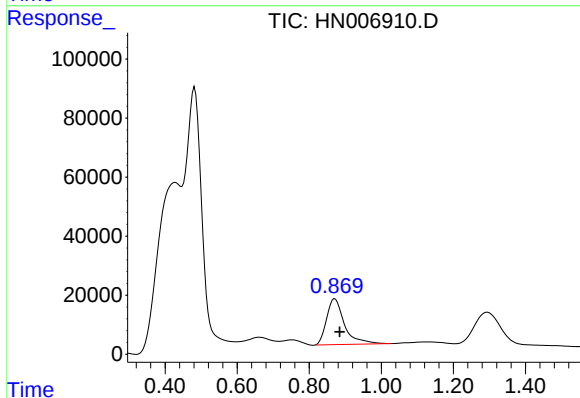


#2 HMX

R.T.: 0.871 min
Delta R.T.: -0.013 min
Response: 533847
Conc: 126.73 ug/L

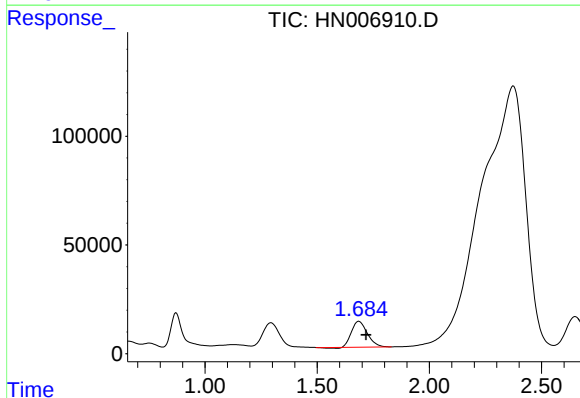


#3 RDX

R.T.: 1.686 min
Delta R.T.: -0.031 min
Response: 577172
Conc: 114.13 ug/L

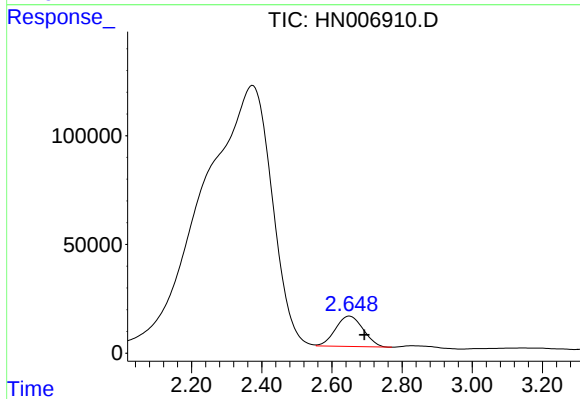

#4 1,3,5-Trinitrobenzene

R.T.: 2.650 min
Delta R.T.: -0.042 min
Response: 765505
Conc: 75.14 ug/L

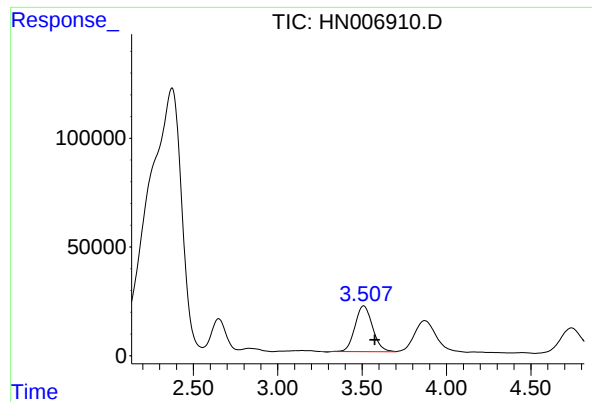

#5 1,3-Dinitrobenzene

R.T.: 3.509 min
Delta R.T.: -0.065 min
Response: 1524495
Conc: 95.56 ng/ml

Instrument :
HPLC_N
ClientSampleId :
YS19-SD01-1014MSD