

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
 Data File : HN006929.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 01-Nov-2014, 12:56
 Operator : TP
 Sample : F4379-01MS
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 YS19-SS32-1014MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 04:08:42 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
 Quant Title :
 QLast Update : Sat Mar 07 03:03:02 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.303	545621	156.325 ug/L
Target Compounds			
2) T HMX	0.873	544655	129.294 ug/L
3) T RDX	1.694	625158	123.617 ug/L
4) T 1,3,5-Trinitrobenzene	2.668	1189907	116.798 ug/L
5) T 1,3-Dinitrobenzene	3.537	2065199	129.455 ng/ml
6) T 3,5-Dinitroaniline	3.910f	1494745	133.096 ug/L
7) T Nitrobenzene	4.776f	1261488	129.683 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
Data File : HN006929.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 01-Nov-2014, 12:56
Operator : TP
Sample : F4379-01MS
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
YS19-SS32-1014MS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 04:08:42 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Quant Title :
QLast Update : Sat Mar 07 03:03:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

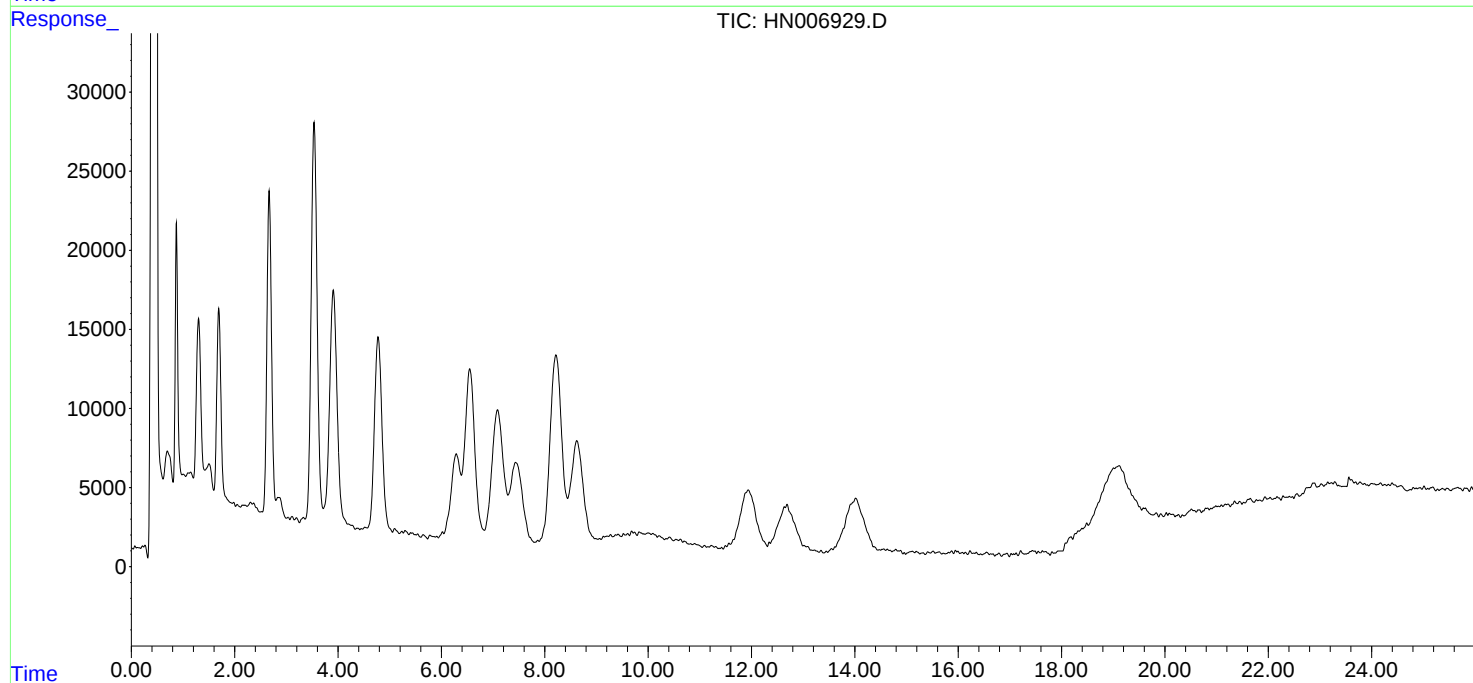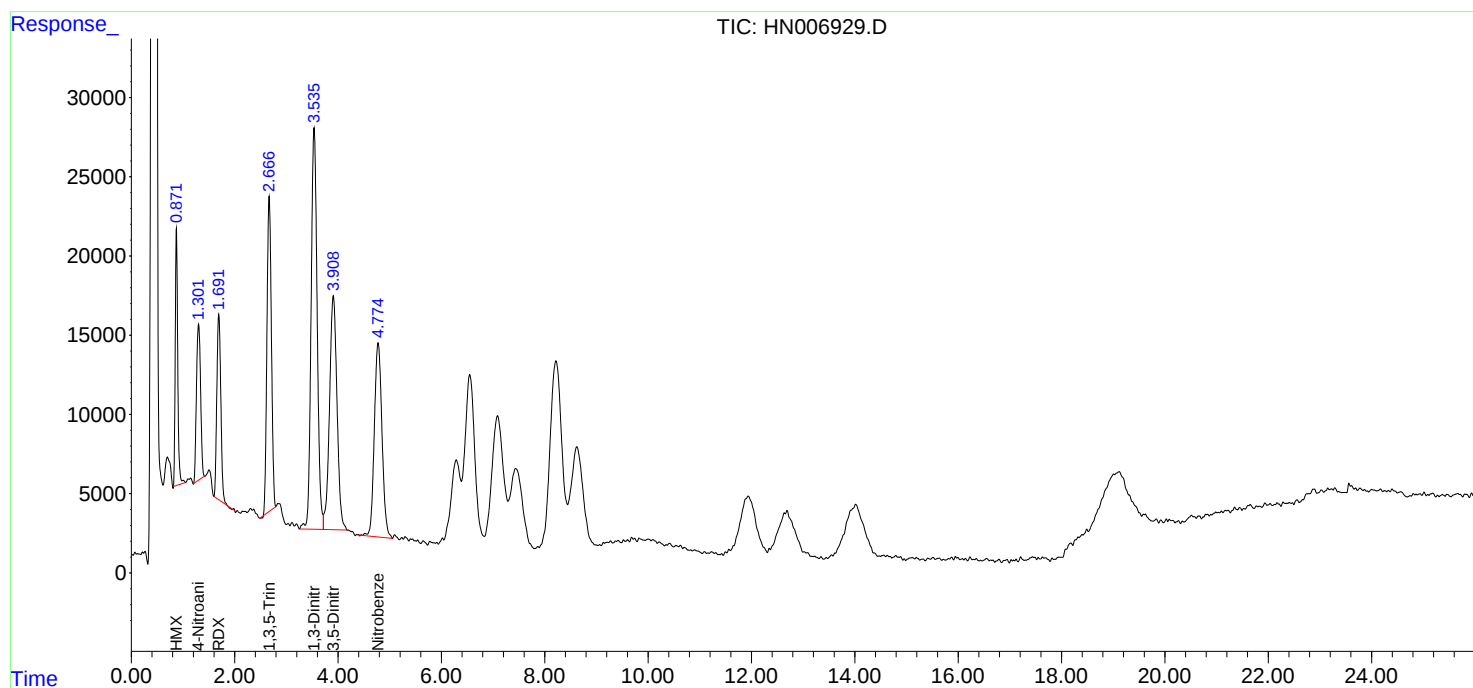


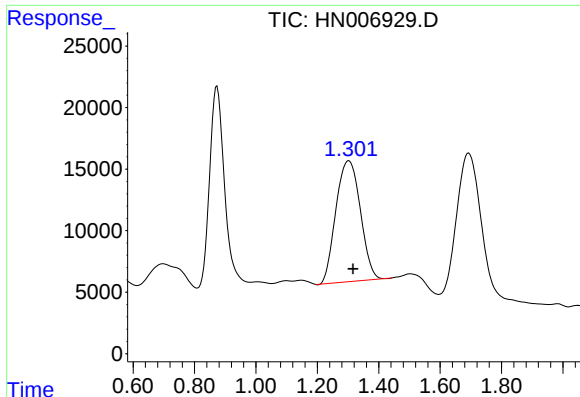

#1 4-Nitroaniline


R.T.: 1.303 min
Delta R.T.: -0.014 min
Response: 545621
Conc: 156.33 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-SS32-1014MS

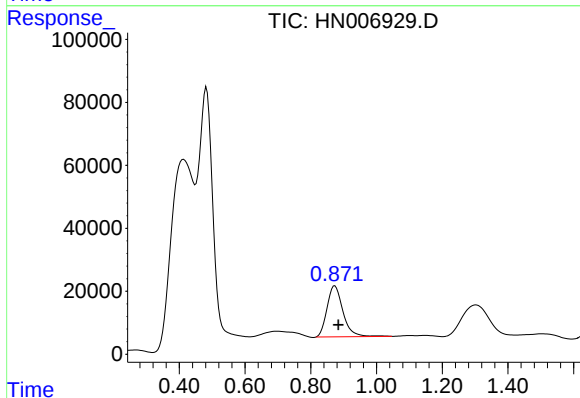


#2 HMX

R.T.: 0.873 min
Delta R.T.: -0.011 min
Response: 544655
Conc: 129.29 ug/L

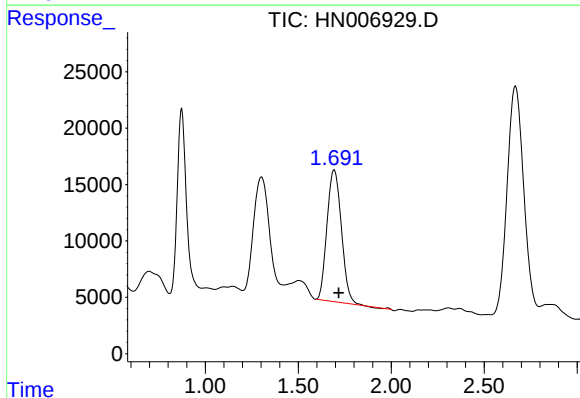


#3 RDX

R.T.: 1.694 min
Delta R.T.: -0.024 min
Response: 625158
Conc: 123.62 ug/L

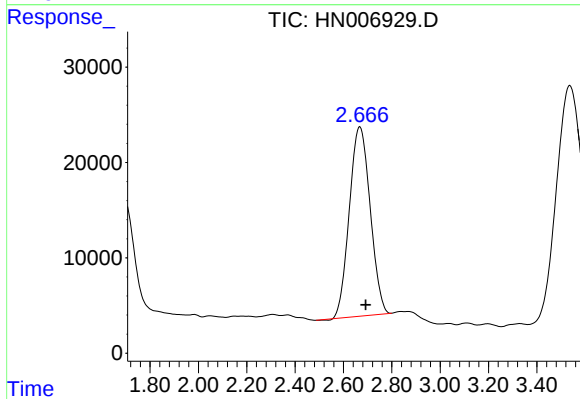

#4 1,3,5-Trinitrobenzene


R.T.: 2.668 min
Delta R.T.: -0.024 min
Response: 1189907
Conc: 116.80 ug/L

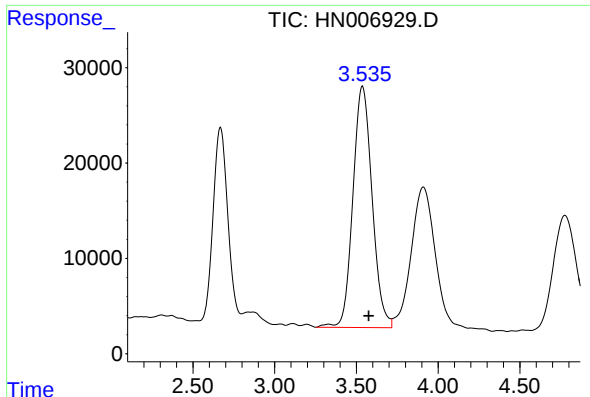

#5 1,3-Dinitrobenzene


R.T.: 3.537 min
Delta R.T.: -0.038 min
Response: 2065199
Conc: 129.45 ng/ml

Instrument :
HPLC_N
ClientSampleId :
YS19-SS32-1014MS

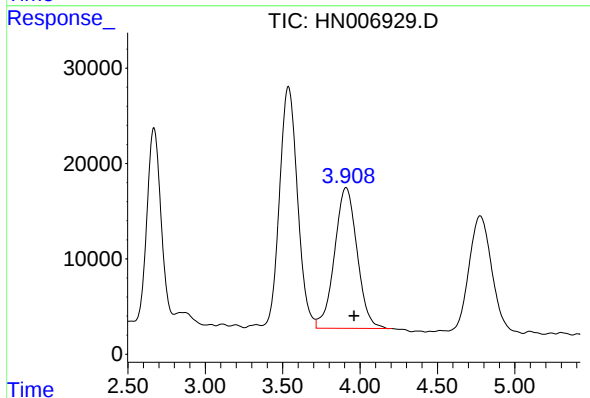

#6 3,5-Dinitroaniline

R.T.: 3.910 min
Delta R.T.: -0.052 min
Response: 1494745
Conc: 133.10 ug/L

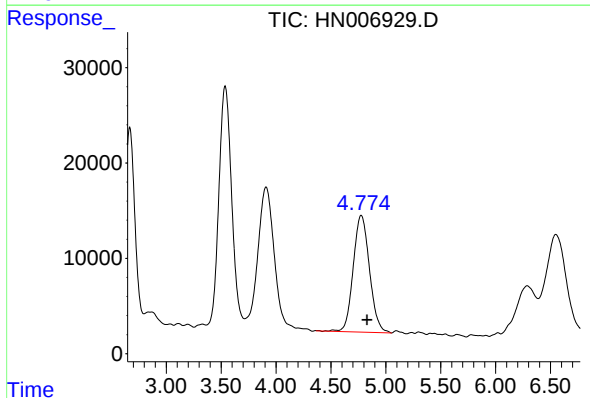

#7 Nitrobenzene

R.T.: 4.776 min
Delta R.T.: -0.054 min
Response: 1261488
Conc: 129.68 ug/L