

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
 Data File : HN006932.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 01-Nov-2014, 14:20
 Operator : TP
 Sample : HSTDCCC0500
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDCCC0500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 04:09:05 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
 Quant Title :
 QLast Update : Sat Mar 07 03:03:02 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.302	1532868	439.180 ug/L
Target Compounds			
2) T HMX	0.874	2015447	478.442 ug/L
3) T RDX	1.687	2560288	506.266 ug/L
4) T 1,3,5-Trinitrobenzene	2.660	5328303	523.012 ug/L
5) T 1,3-Dinitrobenzene	3.523f	8114787	508.667 ng/ml
6) T 3,5-Dinitroaniline	3.893f	5808364	517.191 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
Data File : HN006932.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 01-Nov-2014, 14:20
Operator : TP
Sample : HSTDCCC0500
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 04:09:05 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Quant Title :
QLast Update : Sat Mar 07 03:03:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

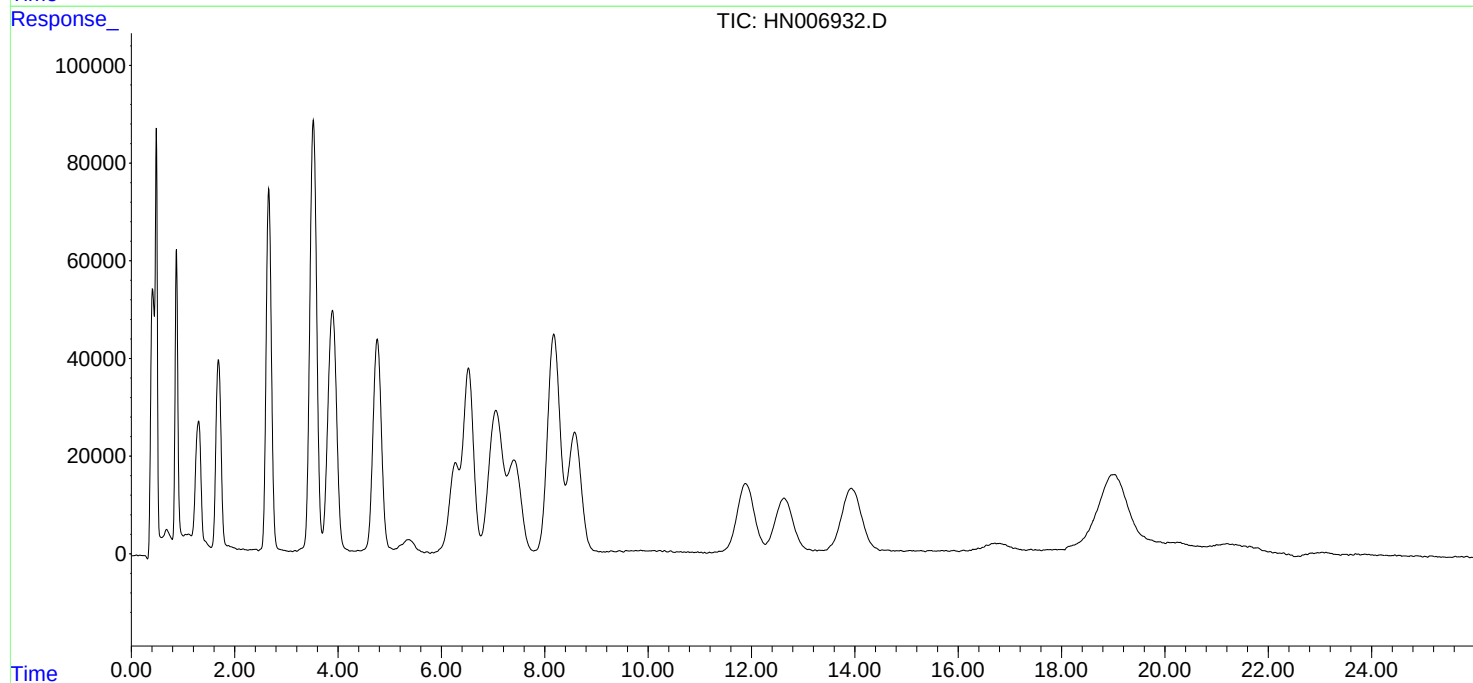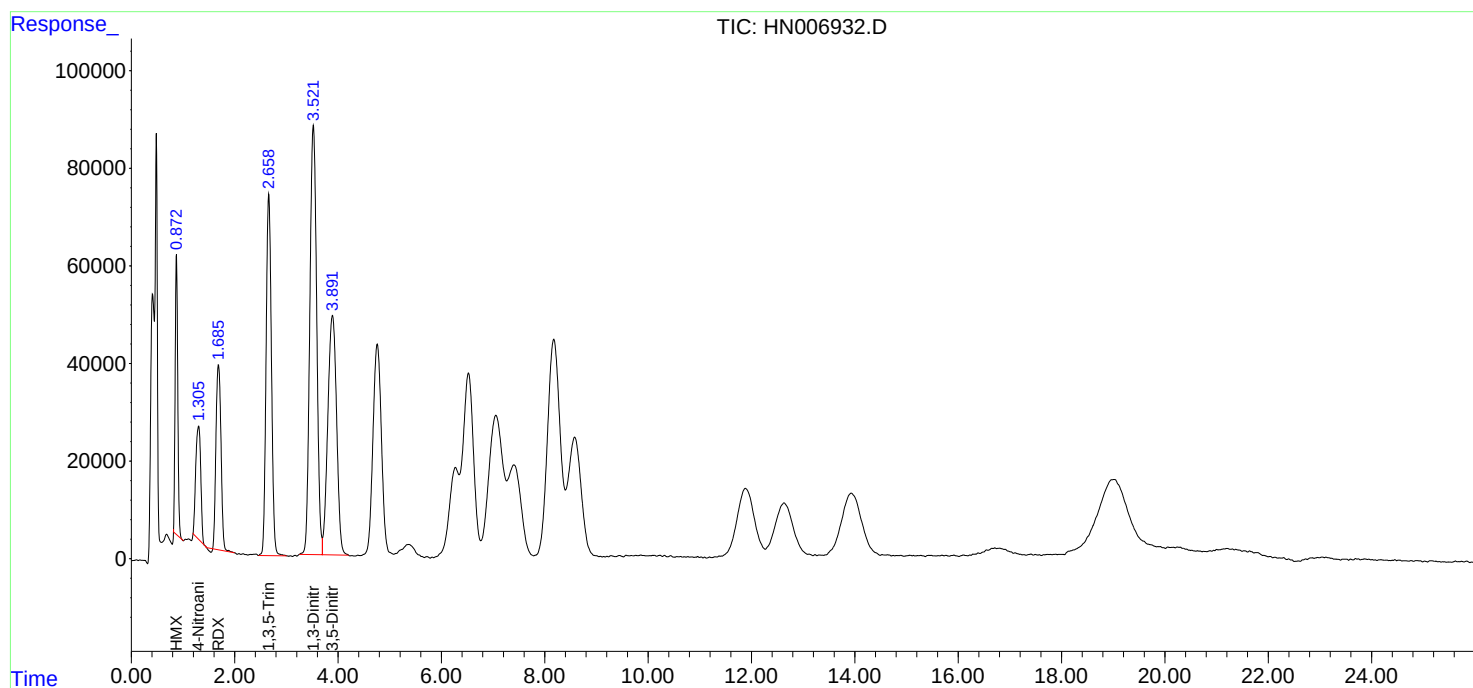


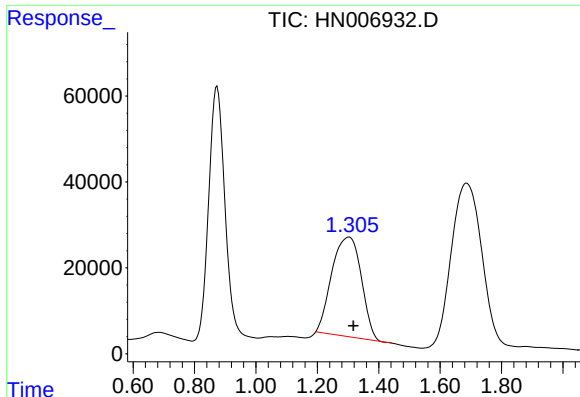

#1 4-Nitroaniline


R.T.: 1.302 min
Delta R.T.: -0.015 min
Response: 1532868
Conc: 439.18 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

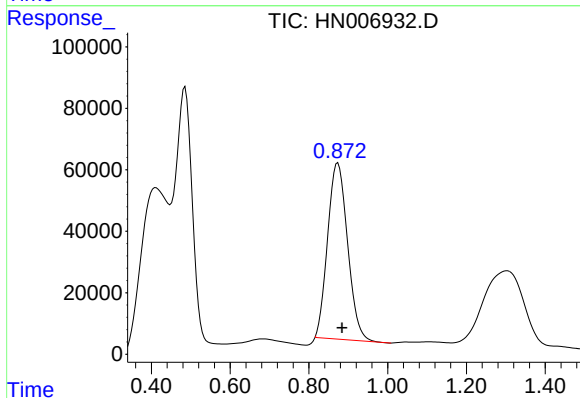


#2 HMX

R.T.: 0.874 min
Delta R.T.: -0.011 min
Response: 2015447
Conc: 478.44 ug/L

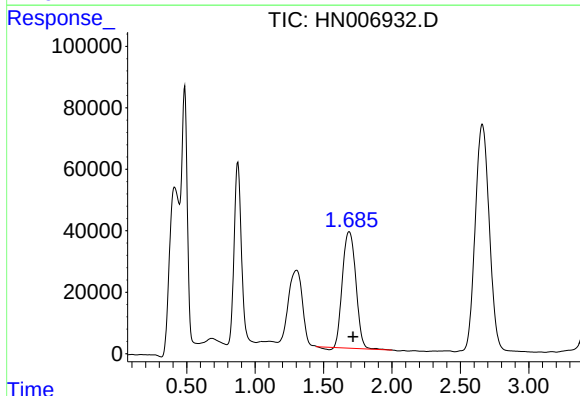


#3 RDX

R.T.: 1.687 min
Delta R.T.: -0.030 min
Response: 2560288
Conc: 506.27 ug/L

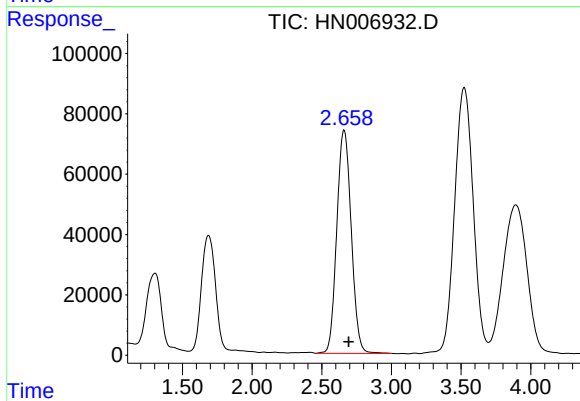

#4 1,3,5-Trinitrobenzene


R.T.: 2.660 min
Delta R.T.: -0.033 min
Response: 5328303
Conc: 523.01 ug/L

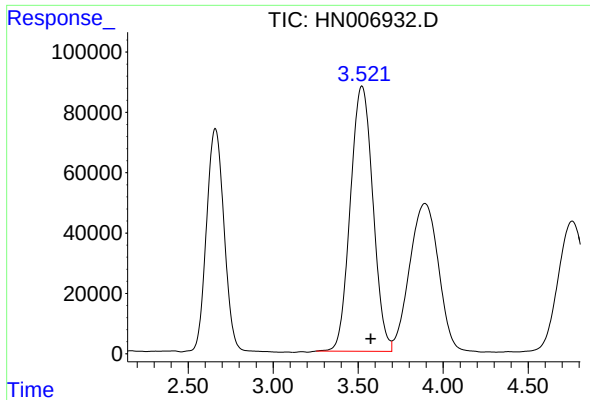

#5 1,3-Dinitrobenzene

R.T.: 3.523 min
Delta R.T.: -0.052 min
Response: 8114787
Conc: 508.67 ng/ml

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

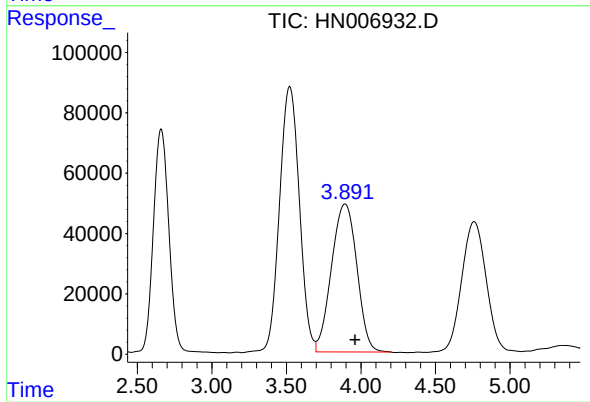

#6 3,5-Dinitroaniline

R.T.: 3.893 min
Delta R.T.: -0.069 min
Response: 5808364
Conc: 517.19 ug/L