

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
Data File : HN006943.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 01-Nov-2014, 19:29
Operator : TP
Sample : HSTDCCC0500
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 04:10:11 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Quant Title :
QLast Update : Sat Mar 07 03:03:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.300	1512610	433.376 ug/L
Target Compounds			
2) T HMX	0.871	1968938	467.402 ug/L
3) T RDX	1.685	2578047	509.777 ug/L
4) T 1,3,5-Trinitrobenzene	2.658	5302380	520.467 ug/L
5) T 1,3-Dinitrobenzene	3.522f	8175218	512.455 ng/ml

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
Data File : HN006943.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 01-Nov-2014, 19:29
Operator : TP
Sample : HSTDCCC0500
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 04:10:11 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Quant Title :
QLast Update : Sat Mar 07 03:03:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

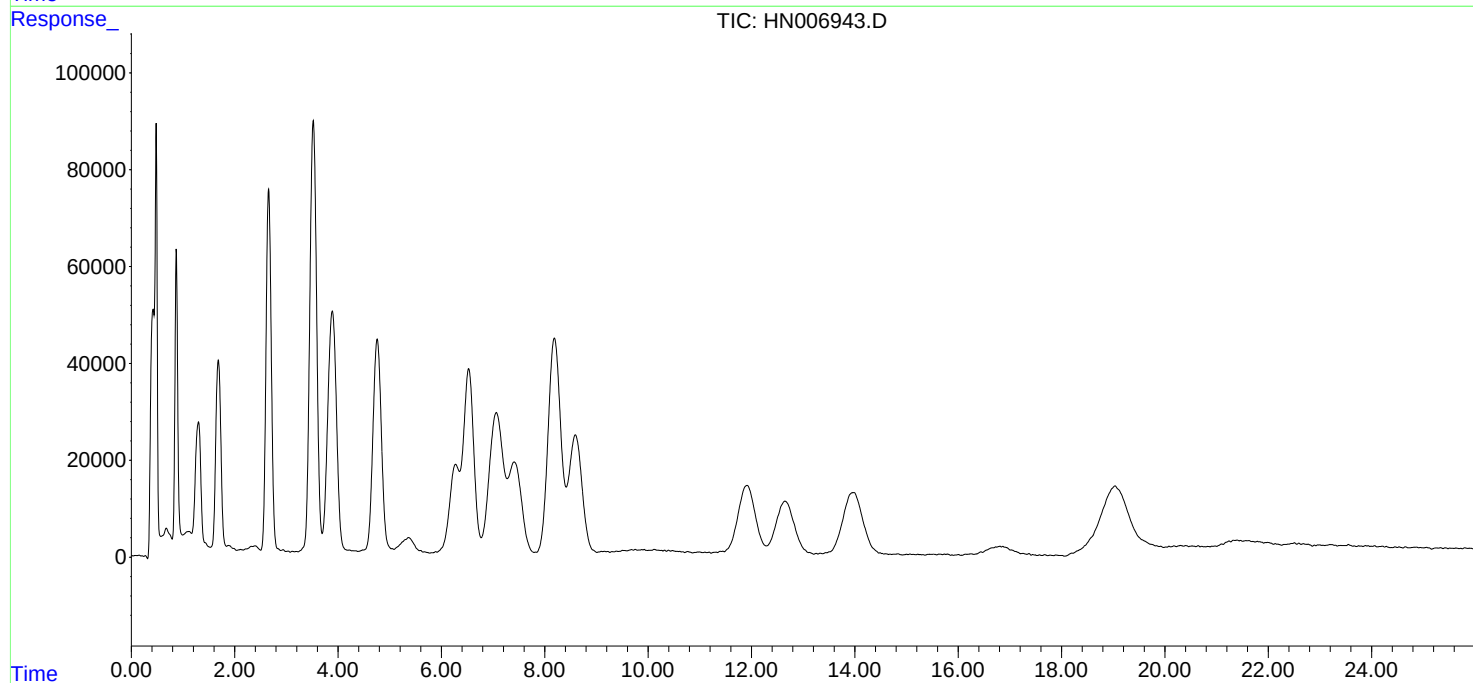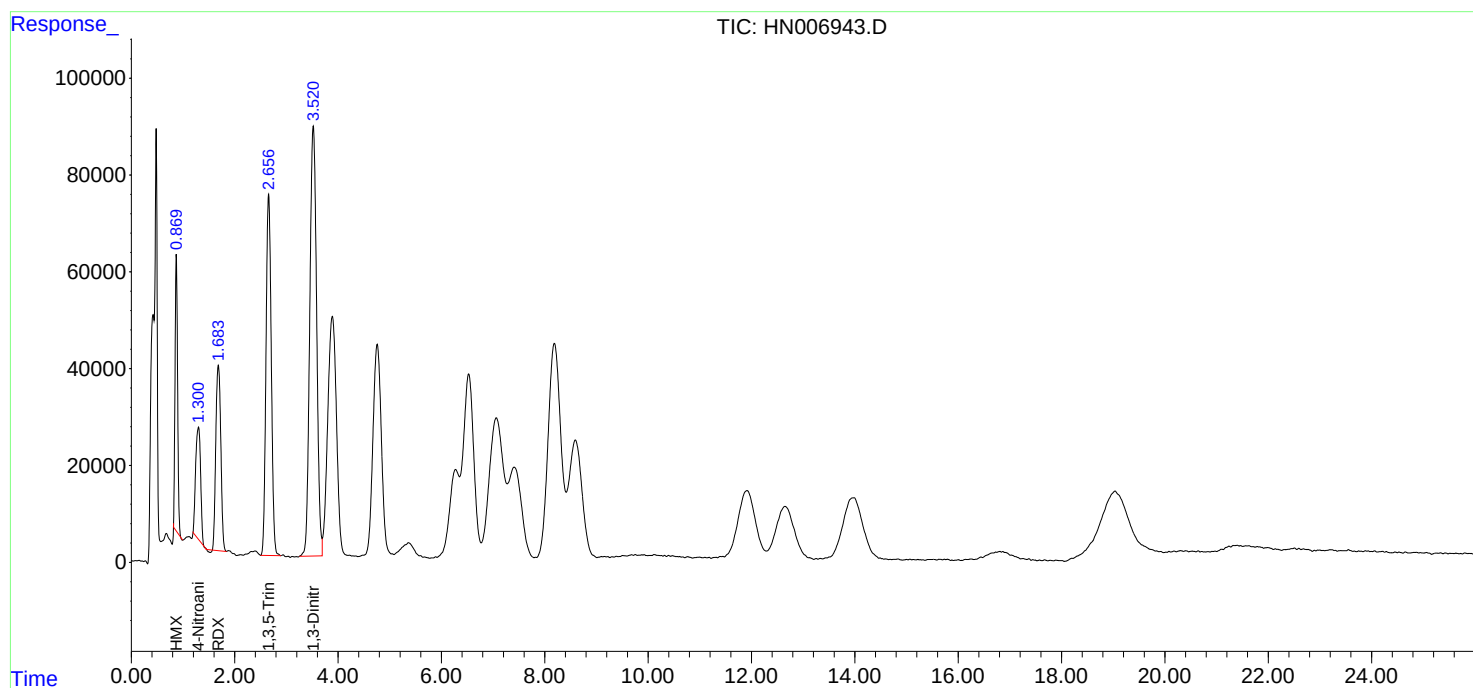


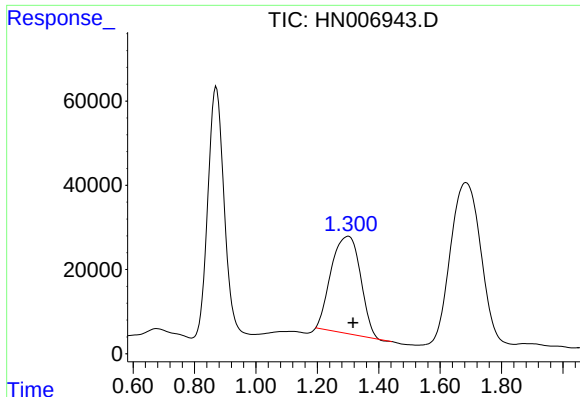

#1 4-Nitroaniline


R.T.: 1.300 min
Delta R.T.: -0.017 min
Response: 1512610
Conc: 433.38 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

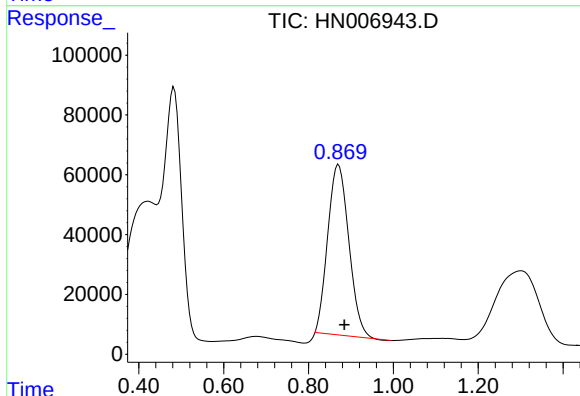


#2 HMX

R.T.: 0.871 min
Delta R.T.: -0.014 min
Response: 1968938
Conc: 467.40 ug/L

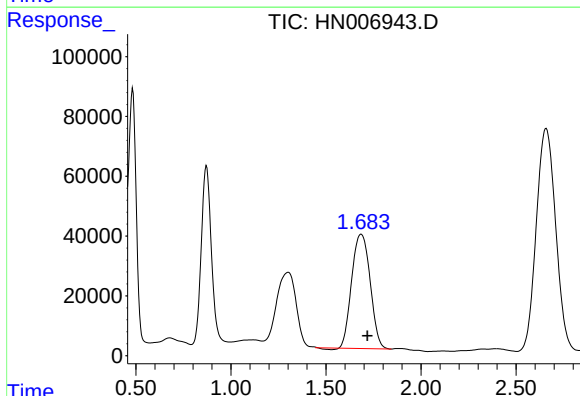


#3 RDX

R.T.: 1.685 min
Delta R.T.: -0.033 min
Response: 2578047
Conc: 509.78 ug/L

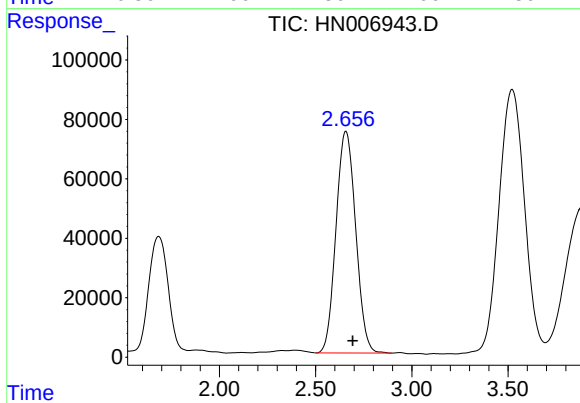

#4 1,3,5-Trinitrobenzene

R.T.: 2.658 min
Delta R.T.: -0.035 min
Response: 5302380
Conc: 520.47 ug/L

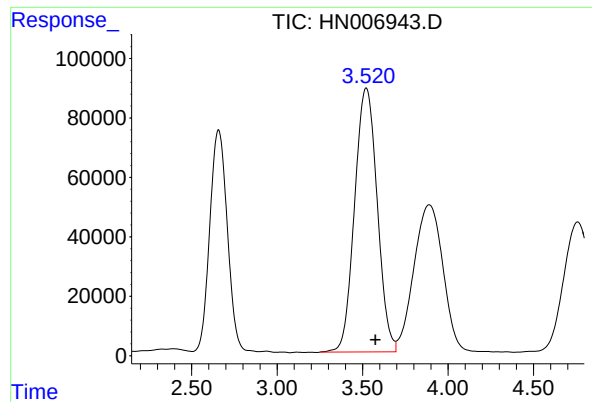

#5 1,3-Dinitrobenzene

R.T.: 3.522 min
Delta R.T.: -0.053 min
Response: 8175218
Conc: 512.46 ng/ml

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500