

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
 Data File : HN006951.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 01-Nov-2014, 23:13
 Operator : TP
 Sample : PB79759BS
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 PB79759BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 04:11:00 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
 Quant Title :
 QLast Update : Sat Mar 07 03:03:02 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.299	566137	162.203 ug/L
Target Compounds			
2) T HMX	0.871	552500	131.157 ug/L
3) T RDX	1.690	739174	146.163 ug/L
4) T 1,3,5-Trinitrobenzene	2.662	1324513	130.011 ug/L
5) T 1,3-Dinitrobenzene	3.532	2167842	135.889 ng/ml
6) T 3,5-Dinitroaniline	3.904f	1563557	139.223 ug/L
7) T Nitrobenzene	4.771f	1243326	127.816 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
Data File : HN006951.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 01-Nov-2014, 23:13
Operator : TP
Sample : PB79759BS
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
PB79759BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 04:11:00 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Quant Title :
QLast Update : Sat Mar 07 03:03:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

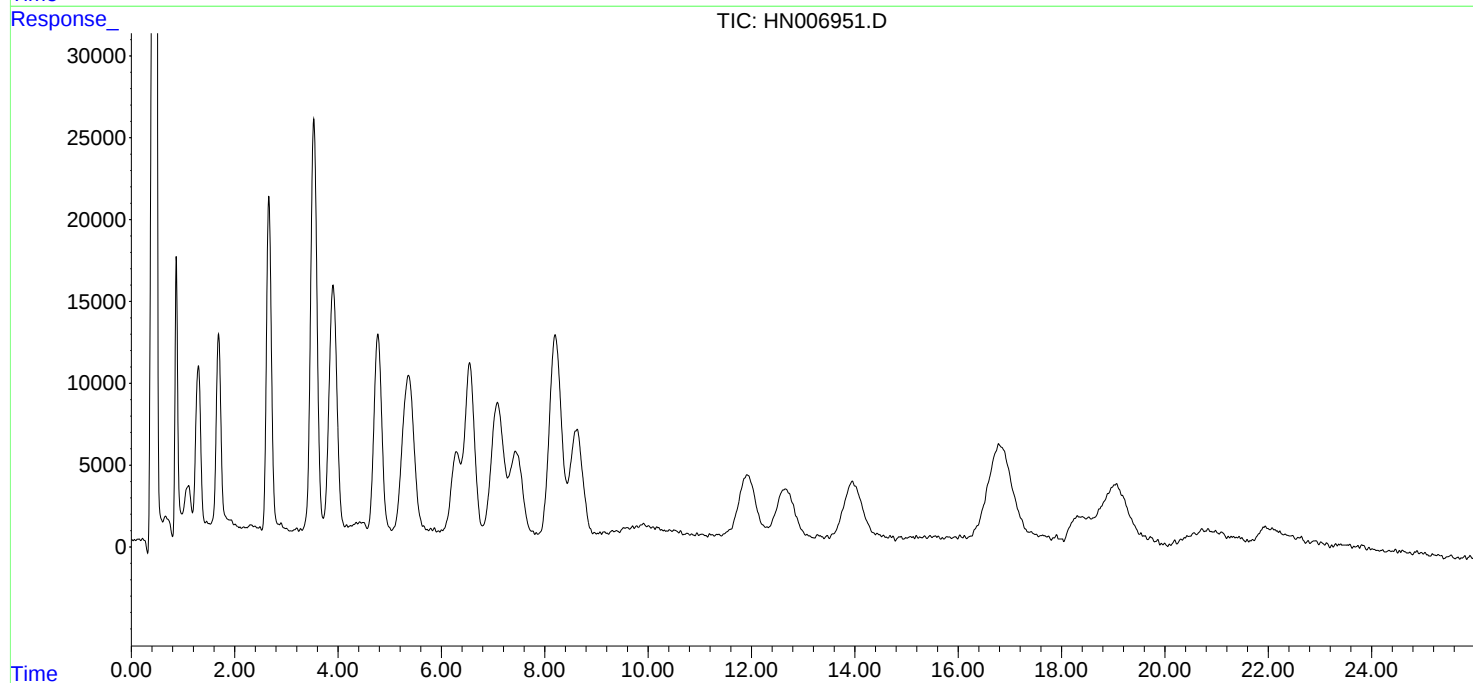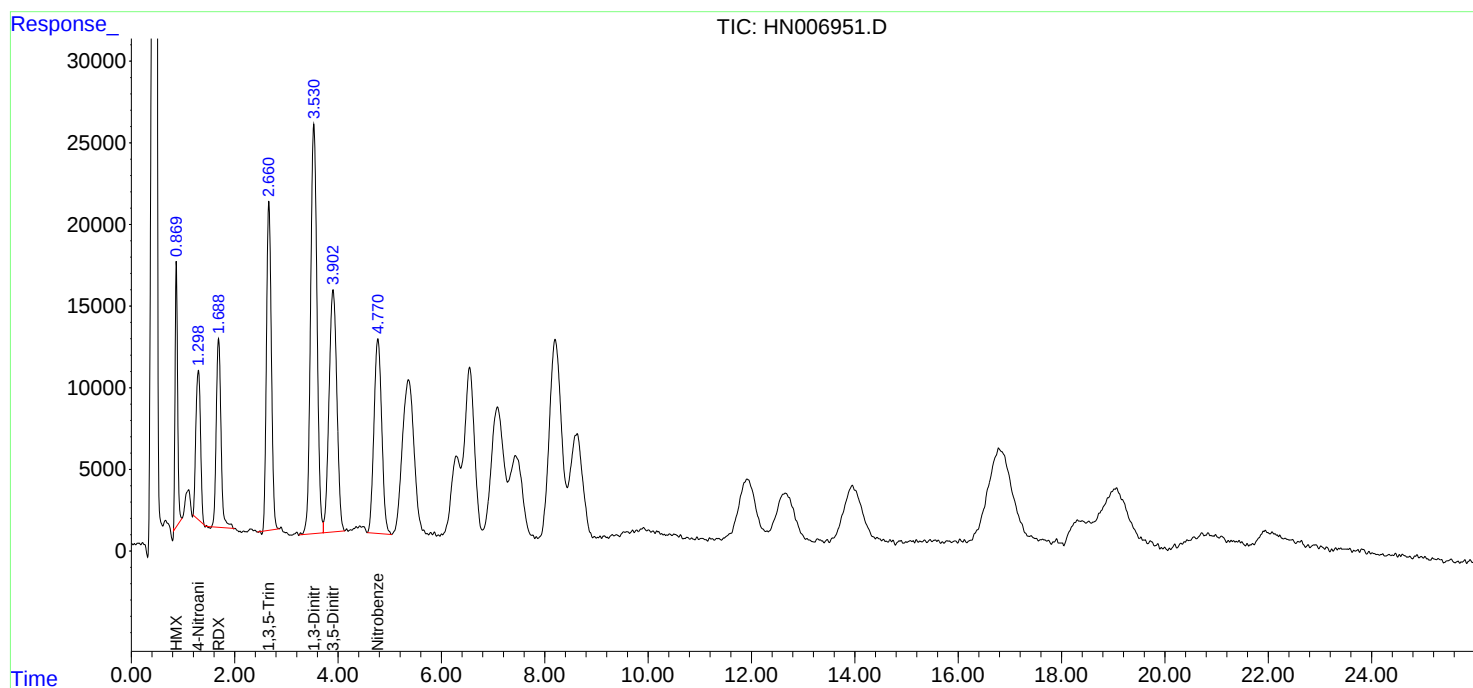


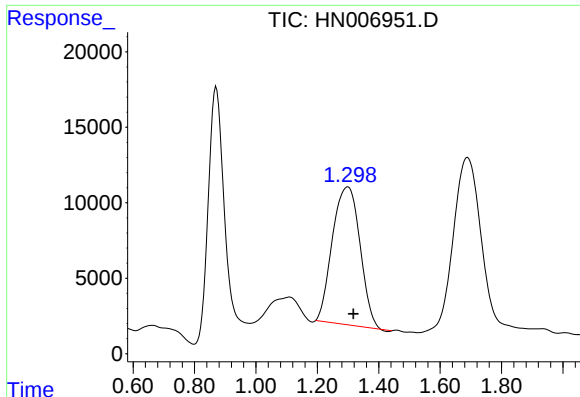

#1 4-Nitroaniline


R.T.: 1.299 min
Delta R.T.: -0.018 min
Response: 566137
Conc: 162.20 ug/L

Instrument :
HPLC_N
ClientSampleId :
PB79759BS

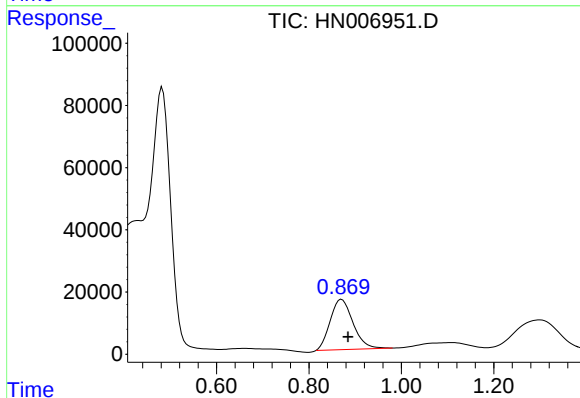


#2 HMX

R.T.: 0.871 min
Delta R.T.: -0.014 min
Response: 552500
Conc: 131.16 ug/L

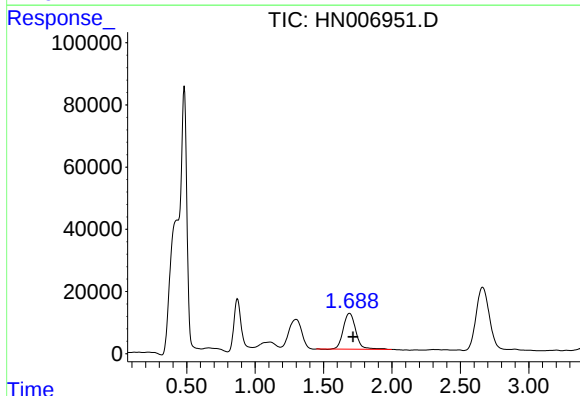


#3 RDX

R.T.: 1.690 min
Delta R.T.: -0.028 min
Response: 739174
Conc: 146.16 ug/L

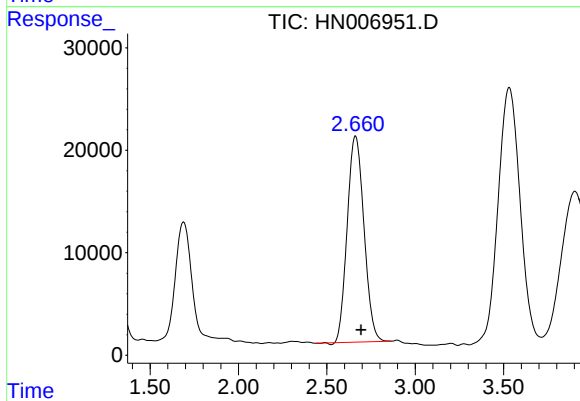

#4 1,3,5-Trinitrobenzene


R.T.: 2.662 min
Delta R.T.: -0.030 min
Response: 1324513
Conc: 130.01 ug/L

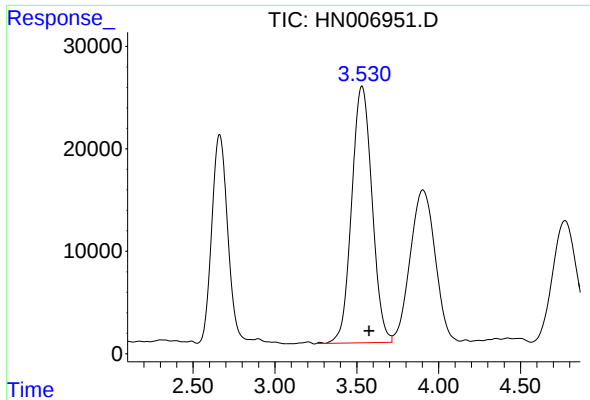

#5 1,3-Dinitrobenzene


R.T.: 3.532 min
Delta R.T.: -0.043 min
Response: 2167842
Conc: 135.89 ng/ml

Instrument :
HPLC_N
ClientSampleId :
PB79759BS

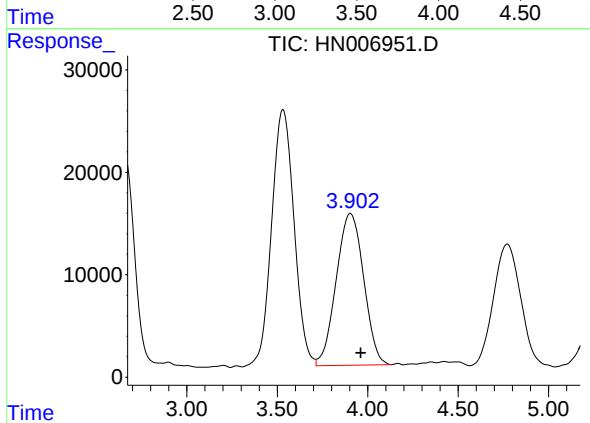

#6 3,5-Dinitroaniline

R.T.: 3.904 min
Delta R.T.: -0.058 min
Response: 1563557
Conc: 139.22 ug/L

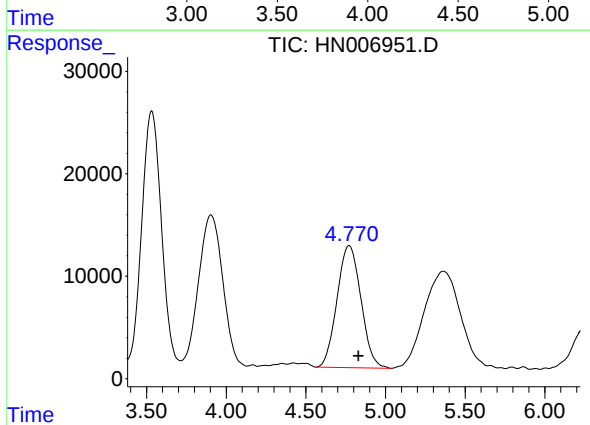

#7 Nitrobenzene

R.T.: 4.771 min
Delta R.T.: -0.059 min
Response: 1243326
Conc: 127.82 ug/L