

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
 Data File : HN006952.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 01-Nov-2014, 23:41
 Operator : TP
 Sample : PB79747BS
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 PB79747BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 04:11:27 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
 Quant Title :
 QLast Update : Sat Mar 07 03:03:02 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.298	604149	173.094 ug/L
Target Compounds			
2) T HMX	0.871	584565	138.769 ug/L
3) T RDX	1.690	755066	149.305 ug/L
4) T 1,3,5-Trinitrobenzene	2.663	1408969	138.301 ug/L
5) T 1,3-Dinitrobenzene	3.529	2151902	134.890 ng/ml
6) T 3,5-Dinitroaniline	3.900f	1702530	151.597 ug/L
7) T Nitrobenzene	4.765f	1262070	129.743 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
Data File : HN006952.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 01-Nov-2014, 23:41
Operator : TP
Sample : PB79747BS
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
PB79747BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 04:11:27 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Quant Title :
QLast Update : Sat Mar 07 03:03:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

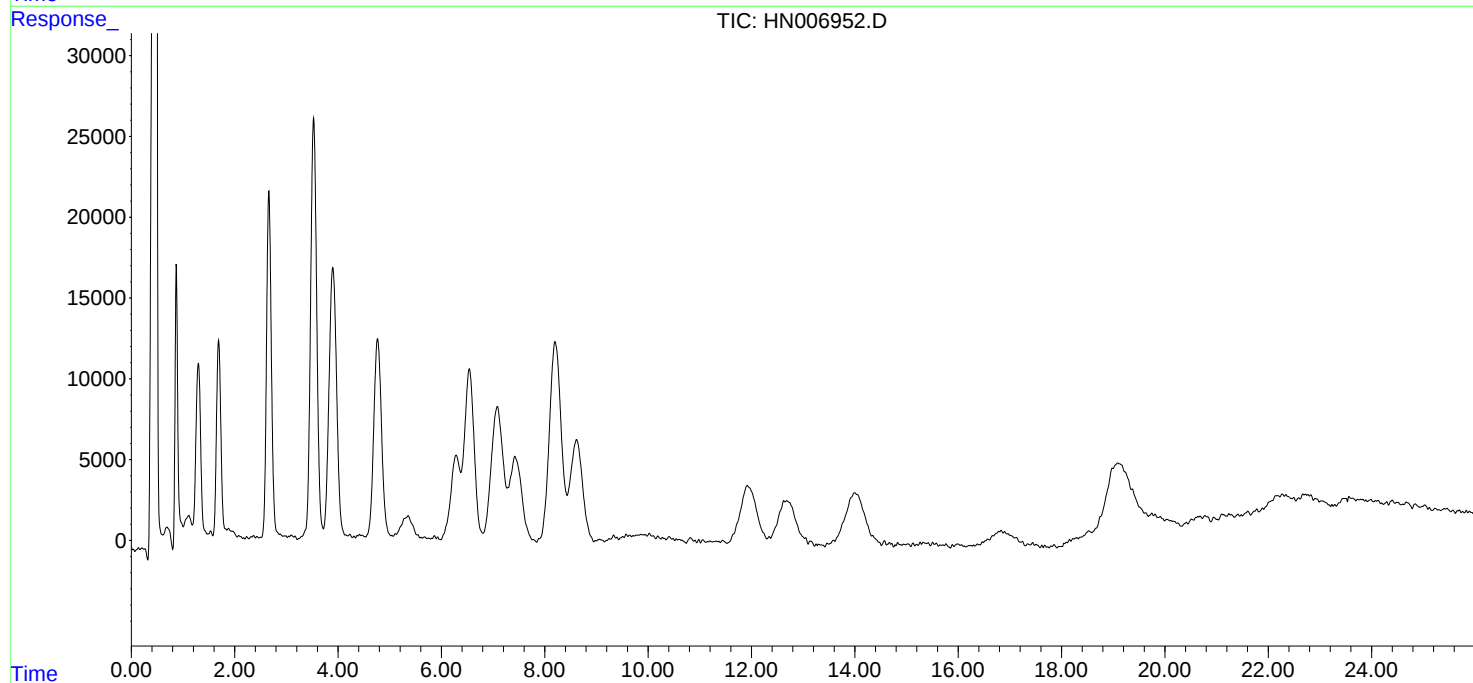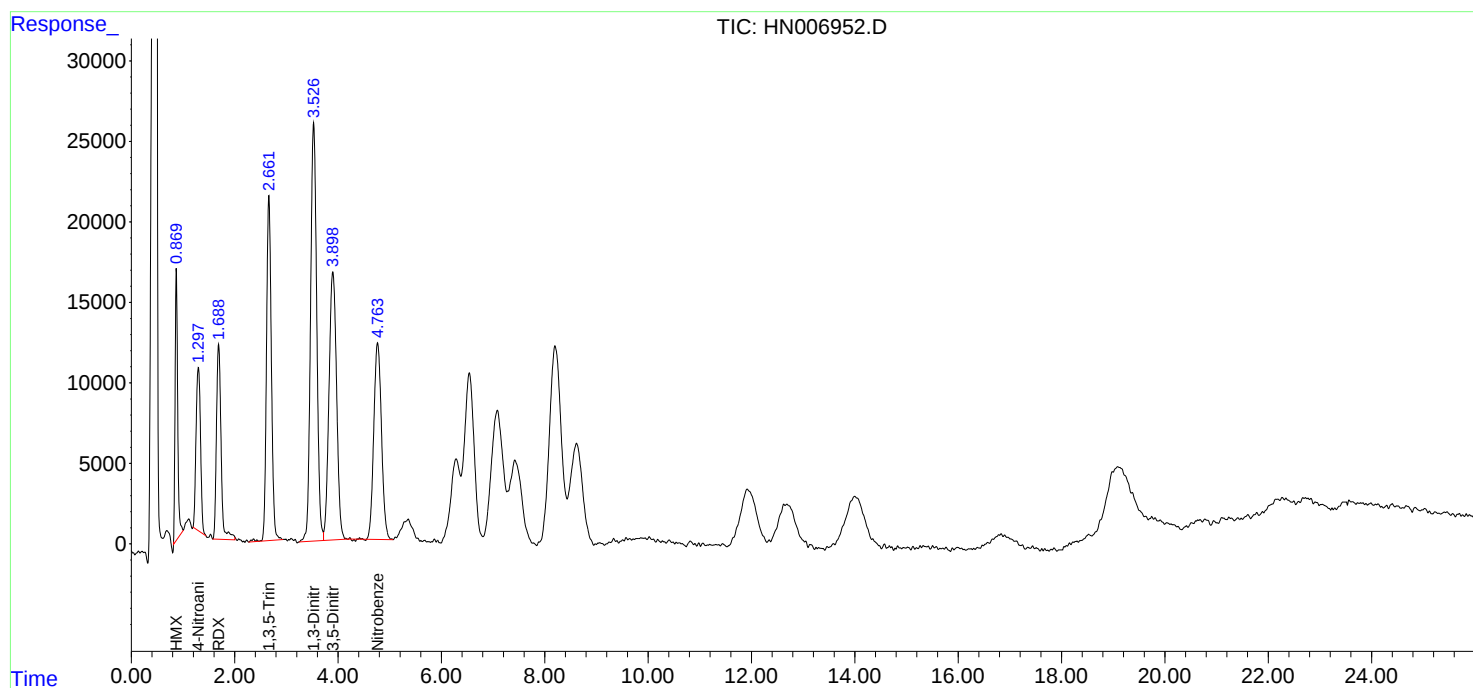


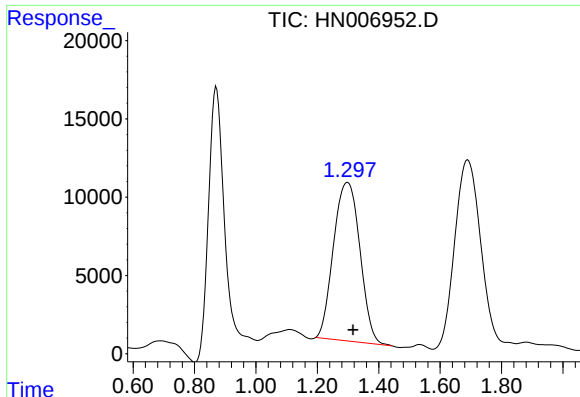

#1 4-Nitroaniline


R.T.: 1.298 min
Delta R.T.: -0.019 min
Response: 604149
Conc: 173.09 ug/L

Instrument :
HPLC_N
ClientSampleId :
PB79747BS

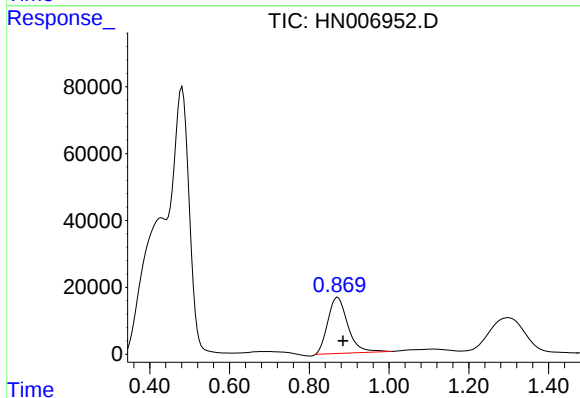


#2 HMX

R.T.: 0.871 min
Delta R.T.: -0.013 min
Response: 584565
Conc: 138.77 ug/L

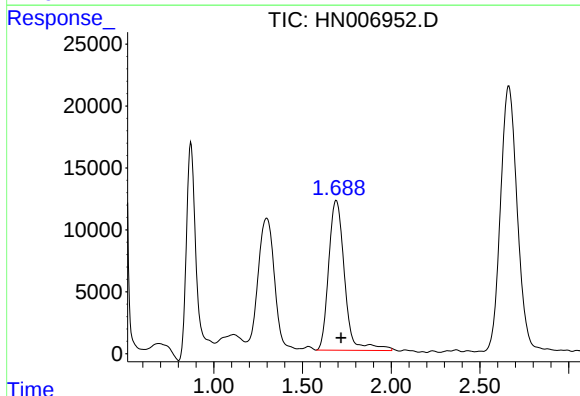


#3 RDX

R.T.: 1.690 min
Delta R.T.: -0.027 min
Response: 755066
Conc: 149.31 ug/L

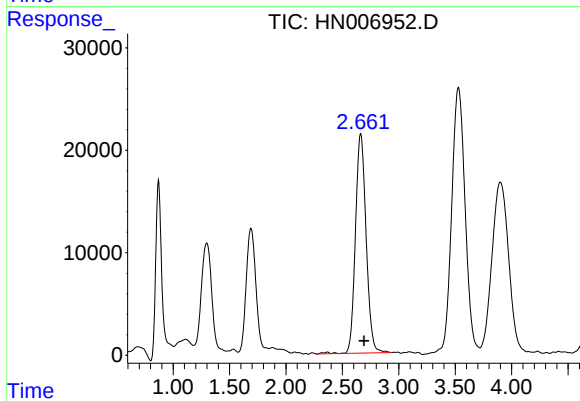

#4 1,3,5-Trinitrobenzene


R.T.: 2.663 min
Delta R.T.: -0.030 min
Response: 1408969
Conc: 138.30 ug/L

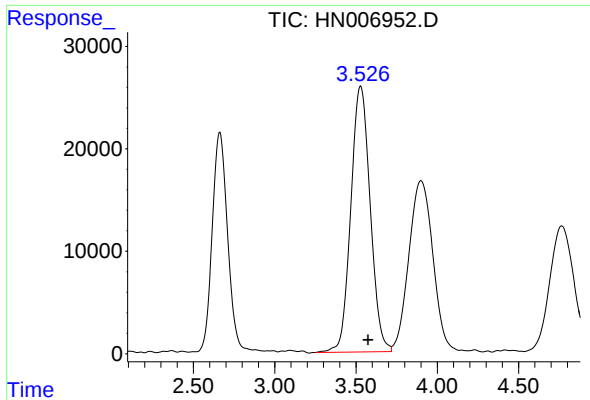

#5 1,3-Dinitrobenzene


R.T.: 3.529 min
Delta R.T.: -0.046 min
Response: 2151902
Conc: 134.89 ng/ml

Instrument :
HPLC_N
ClientSampleId :
PB79747BS

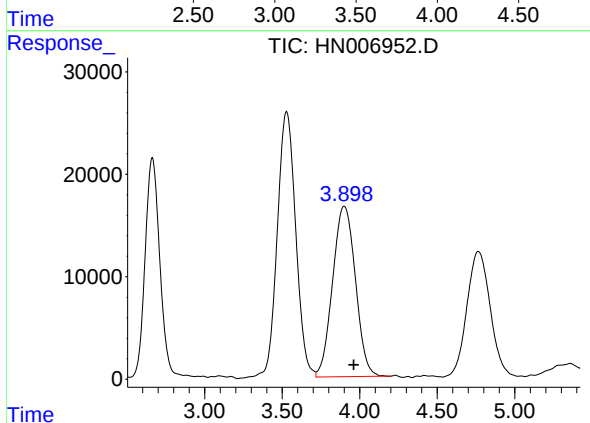

#6 3,5-Dinitroaniline

R.T.: 3.900 min
Delta R.T.: -0.062 min
Response: 1702530
Conc: 151.60 ug/L

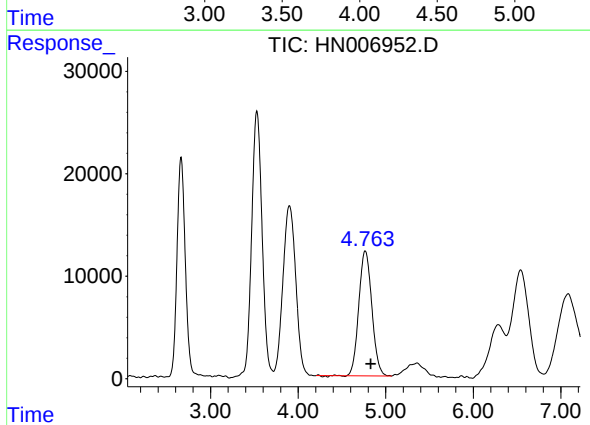

#7 Nitrobenzene

R.T.: 4.765 min
Delta R.T.: -0.065 min
Response: 1262070
Conc: 129.74 ug/L