

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
 Data File : HN006953.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 02-Nov-2014, 00:09
 Operator : TP
 Sample : PB79746BS
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 PB79746BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 04:11:36 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
 Quant Title :
 QLast Update : Sat Mar 07 03:03:02 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.300	586447	168.022 ug/L
Target Compounds			
2) T HMX	0.875	572590	135.926 ug/L
3) T RDX	1.696	721068	142.582 ug/L
4) T 1,3,5-Trinitrobenzene	2.667	1404410	137.853 ug/L
5) T 1,3-Dinitrobenzene	3.533	2160580	135.434 ng/ml
6) T 3,5-Dinitroaniline	3.904f	1691989	150.659 ug/L
7) T Nitrobenzene	4.771f	1273877	130.957 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
Data File : HN006953.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 02-Nov-2014, 00:09
Operator : TP
Sample : PB79746BS
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
PB79746BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 04:11:36 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Quant Title :
QLast Update : Sat Mar 07 03:03:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

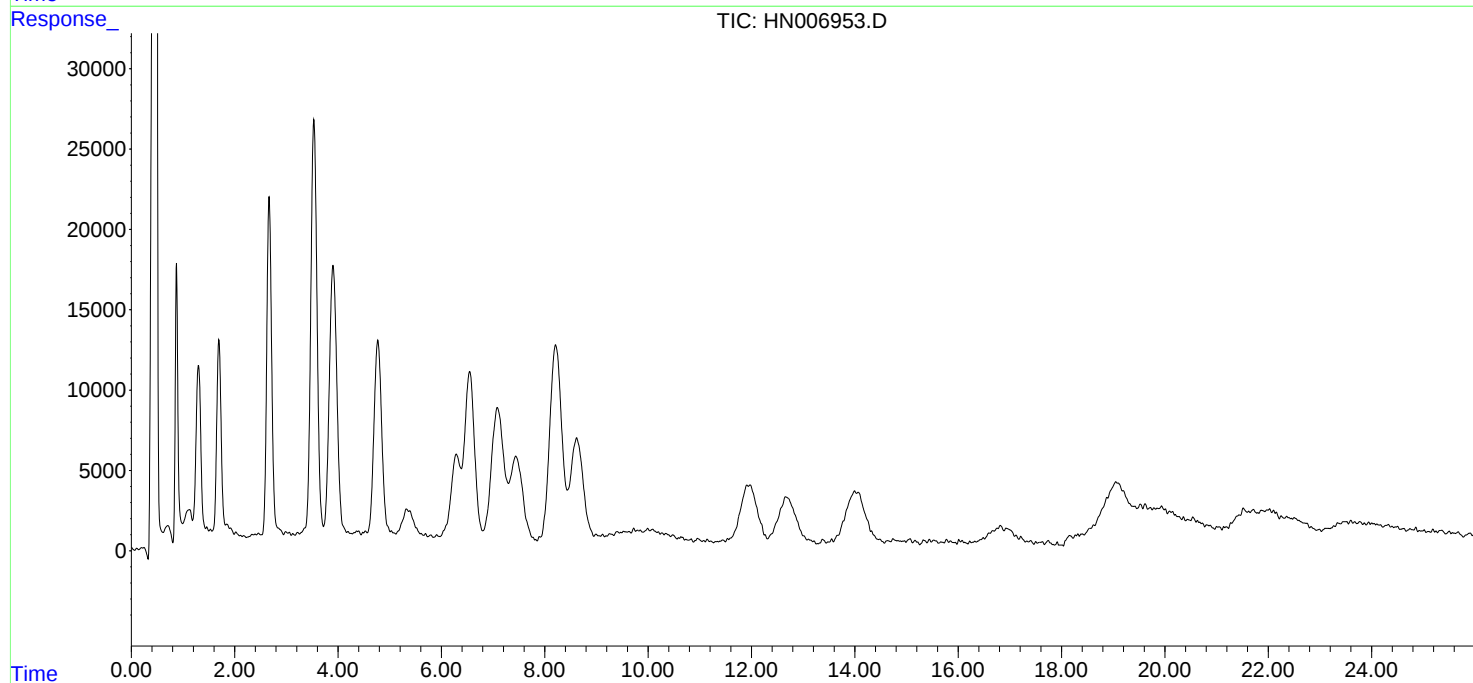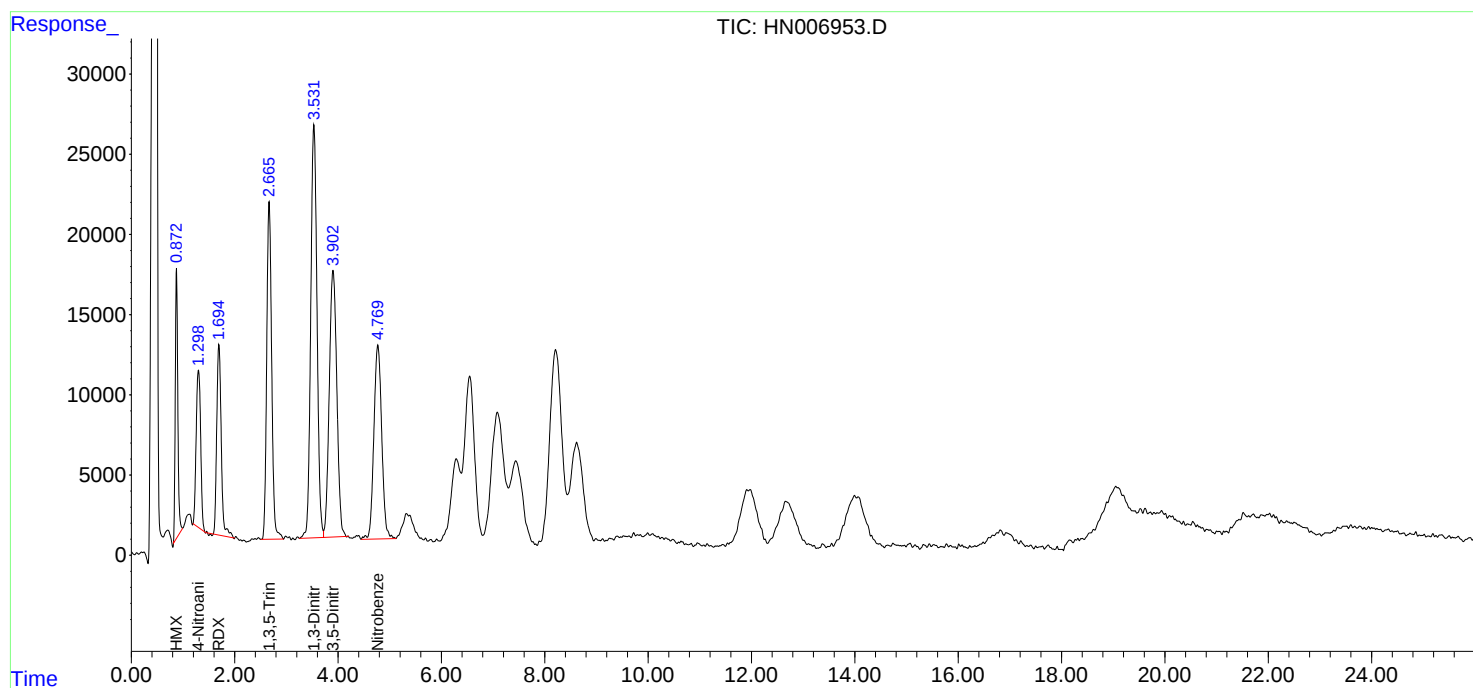


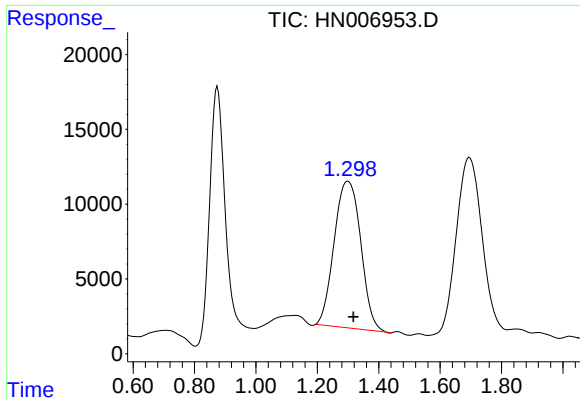

#1 4-Nitroaniline


R.T.: 1.300 min
Delta R.T.: -0.017 min
Response: 586447
Conc: 168.02 ug/L

Instrument :
HPLC_N
ClientSampleId :
PB79746BS

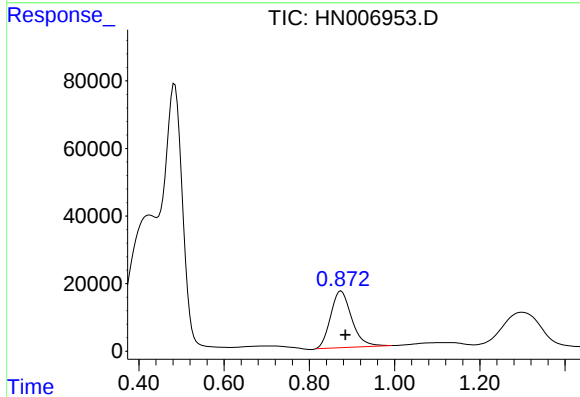


#2 HMX

R.T.: 0.875 min
Delta R.T.: -0.010 min
Response: 572590
Conc: 135.93 ug/L

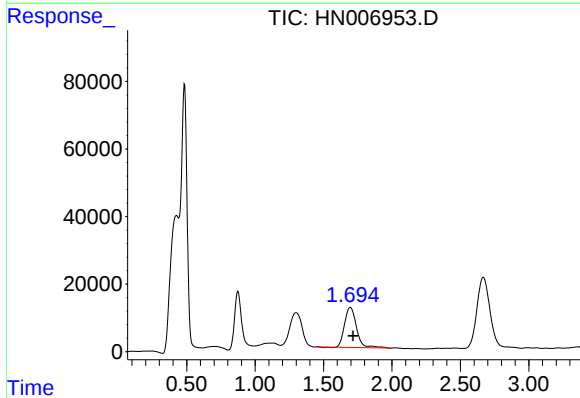


#3 RDX

R.T.: 1.696 min
Delta R.T.: -0.022 min
Response: 721068
Conc: 142.58 ug/L

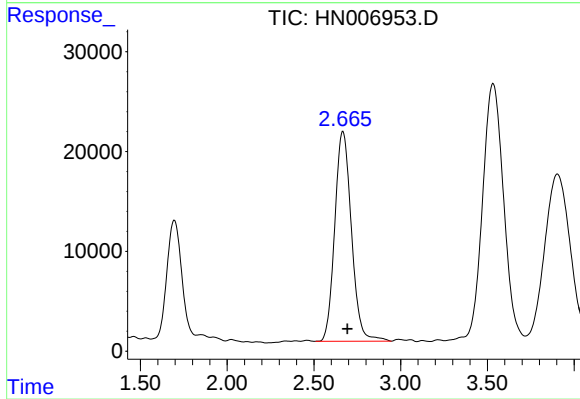

#4 1,3,5-Trinitrobenzene


R.T.: 2.667 min
Delta R.T.: -0.025 min
Response: 1404410
Conc: 137.85 ug/L

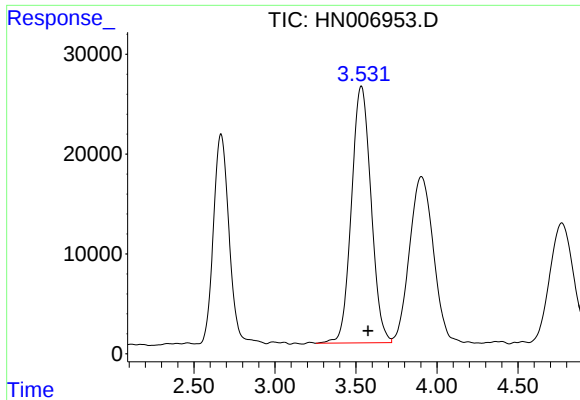

#5 1,3-Dinitrobenzene


R.T.: 3.533 min
Delta R.T.: -0.041 min
Response: 2160580
Conc: 135.43 ng/ml

Instrument :
HPLC_N
ClientSampleId :
PB79746BS

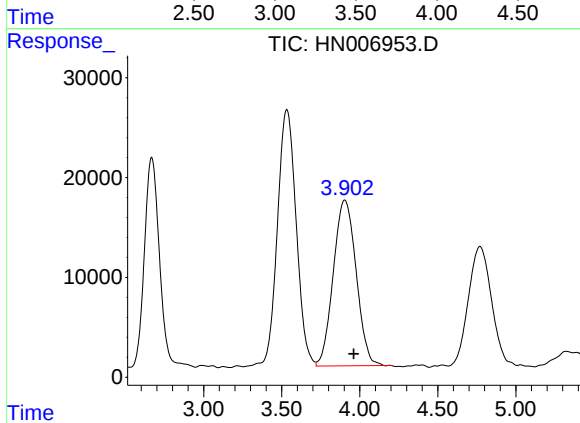

#6 3,5-Dinitroaniline

R.T.: 3.904 min
Delta R.T.: -0.058 min
Response: 1691989
Conc: 150.66 ug/L

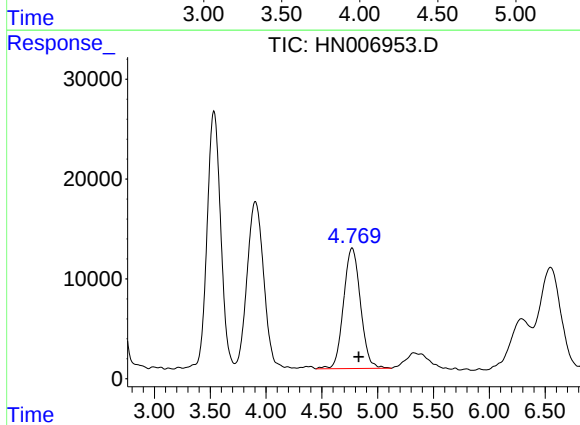

#7 Nitrobenzene

R.T.: 4.771 min
Delta R.T.: -0.060 min
Response: 1273877
Conc: 130.96 ug/L