

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
 Data File : HN006954.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 02-Nov-2014, 00:37
 Operator : TP
 Sample : HSTDCCC0500
 Misc :
 ALS Vial : 74 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 HSTDCCC0500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 04:11:45 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
 Quant Title :
 QLast Update : Sat Mar 07 03:03:02 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.299	1496640	428.801 ug/L
Target Compounds			
2) T HMX	0.872	1997455	474.171 ug/L
3) T RDX	1.684	2622676	518.602 ug/L
4) T 1,3,5-Trinitrobenzene	2.658	5324573	522.645 ug/L
5) T 1,3-Dinitrobenzene	3.523f	8177178	512.578 ng/ml
6) T 3,5-Dinitroaniline	3.895f	5840152	520.021 ug/L
7) T Nitrobenzene	4.763f	5031413	517.238 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
Data File : HN006954.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 02-Nov-2014, 00:37
Operator : TP
Sample : HSTDCCC0500
Misc :
ALS Vial : 74 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 04:11:45 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Quant Title :
QLast Update : Sat Mar 07 03:03:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

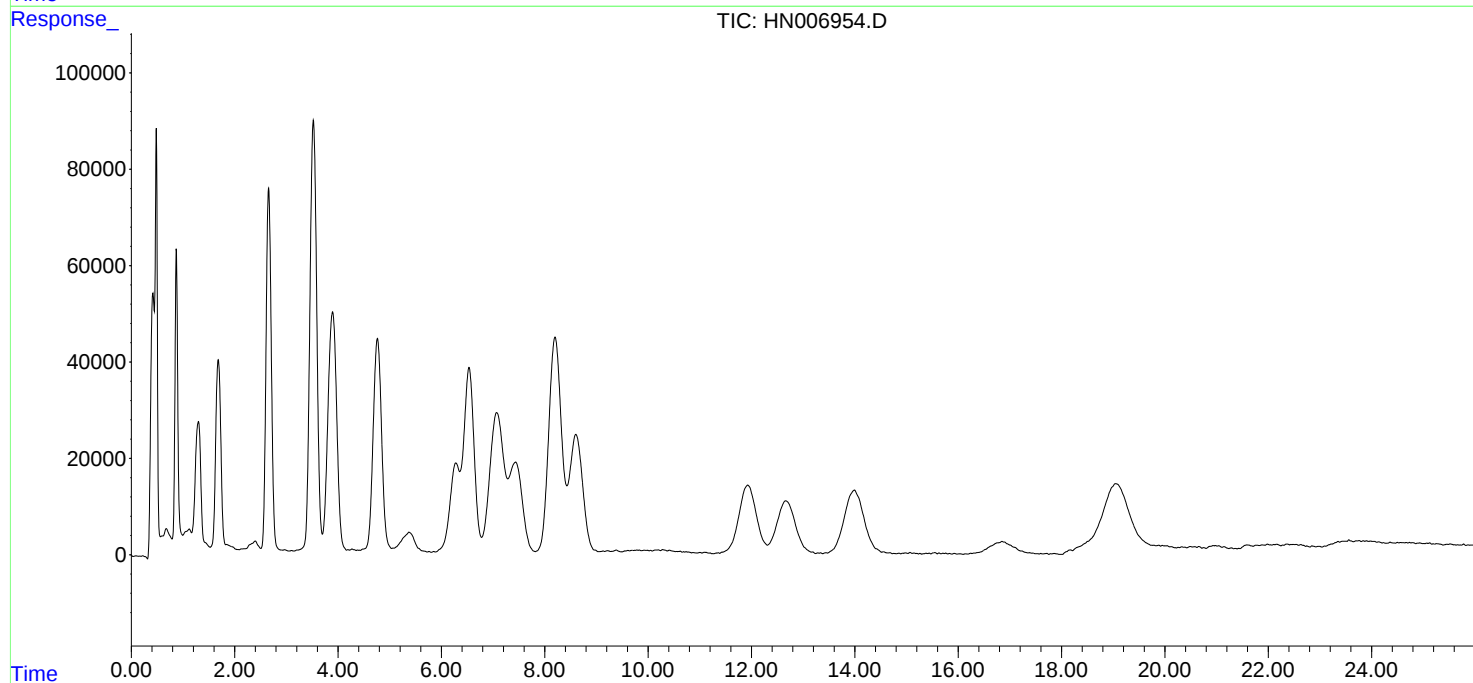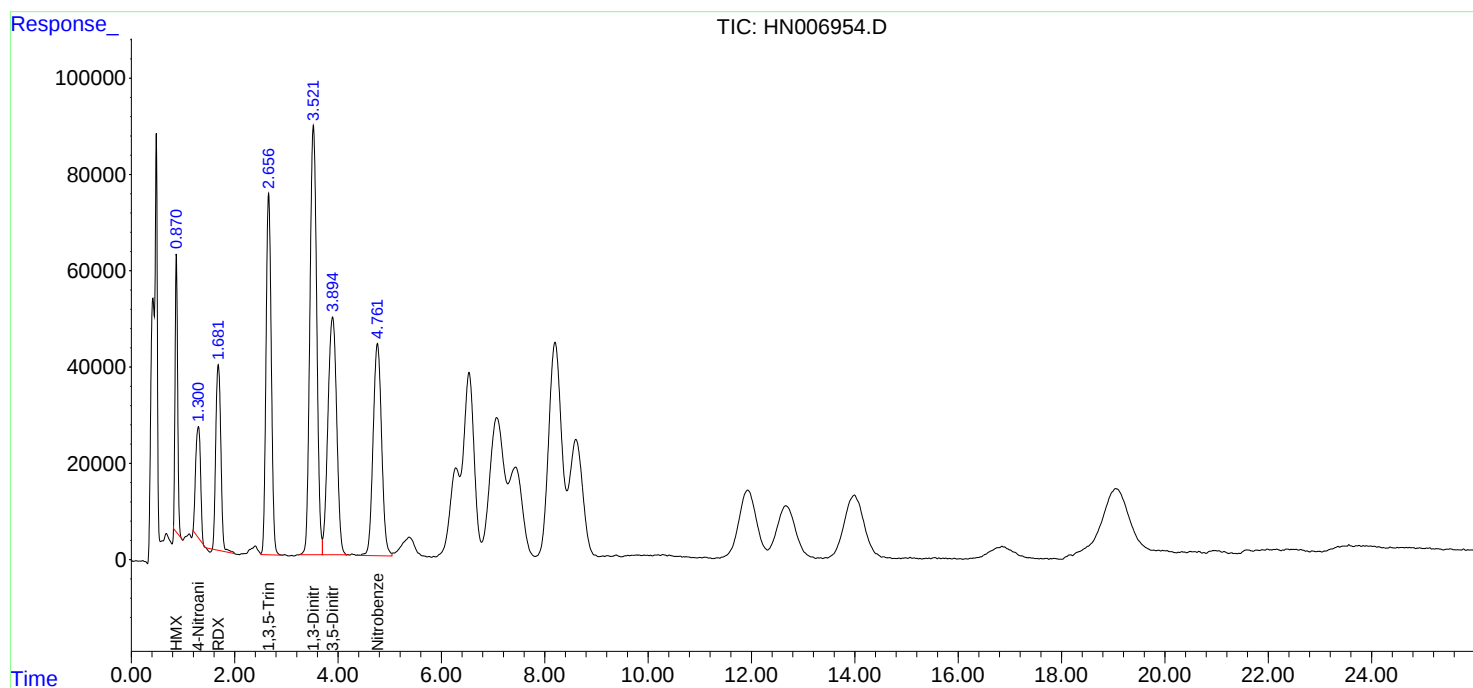


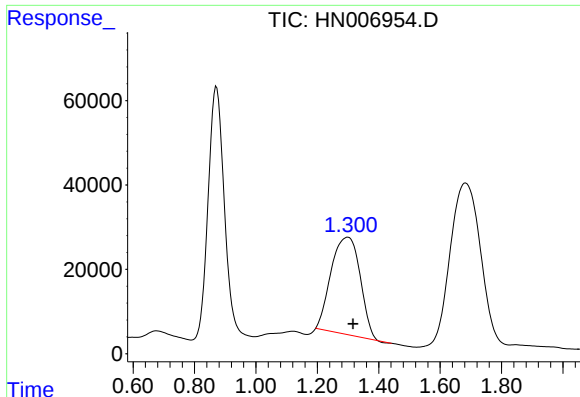

#1 4-Nitroaniline


R.T.: 1.299 min
Delta R.T.: -0.018 min
Response: 1496640
Conc: 428.80 ug/L

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

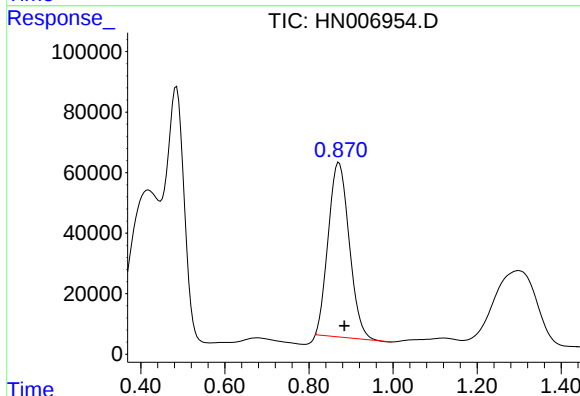


#2 HMX

R.T.: 0.872 min
Delta R.T.: -0.013 min
Response: 1997455
Conc: 474.17 ug/L

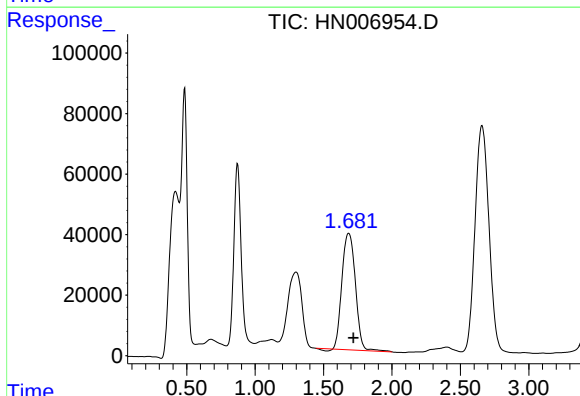


#3 RDX

R.T.: 1.684 min
Delta R.T.: -0.034 min
Response: 2622676
Conc: 518.60 ug/L

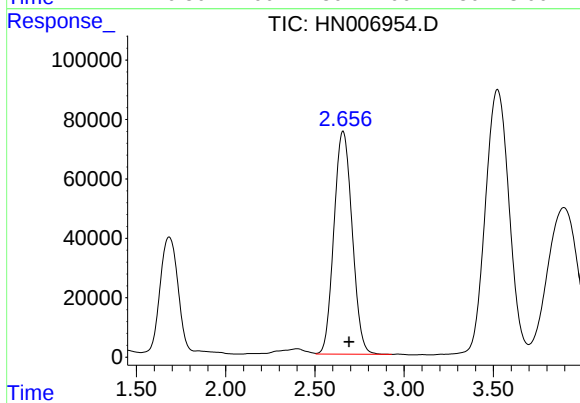

#4 1,3,5-Trinitrobenzene


R.T.: 2.658 min
Delta R.T.: -0.035 min
Response: 5324573
Conc: 522.65 ug/L

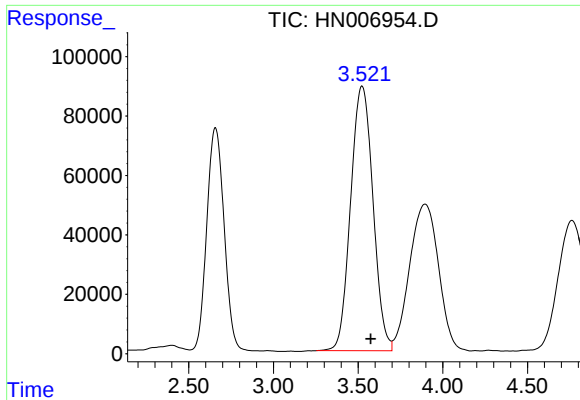

#5 1,3-Dinitrobenzene


R.T.: 3.523 min
Delta R.T.: -0.051 min
Response: 8177178
Conc: 512.58 ng/ml

Instrument :
HPLC_N
ClientSampleId :
HSTDCCC0500

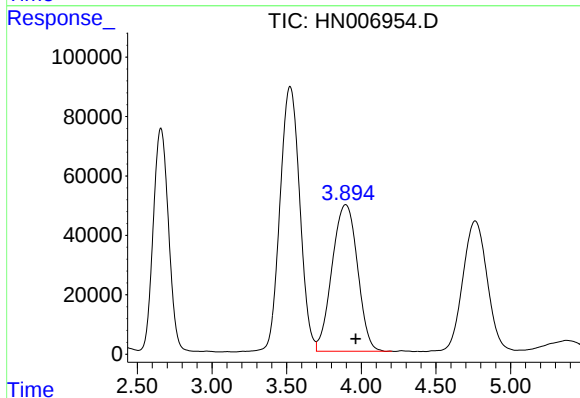

#6 3,5-Dinitroaniline

R.T.: 3.895 min
Delta R.T.: -0.067 min
Response: 5840152
Conc: 520.02 ug/L

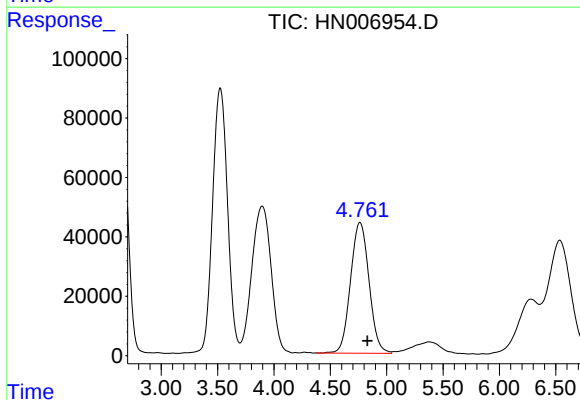

#7 Nitrobenzene

R.T.: 4.763 min
Delta R.T.: -0.068 min
Response: 5031413
Conc: 517.24 ug/L