

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
 Data File : HN006956.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 02-Nov-2014, 01:33
 Operator : TP
 Sample : F4325-03MS
 Misc :
 ALS Vial : 82 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 YS19-SB19-1014MS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 04:11:59 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
 Quant Title :
 QLast Update : Sat Mar 07 03:03:02 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.302	607948	174.182 ug/L
Target Compounds			
2) T HMX	0.874	616690	146.395 ug/L
3) T RDX	1.698	734804	145.298 ug/L
4) T 1,3,5-Trinitrobenzene	2.677	1434278	140.785 ug/L
5) T 1,3-Dinitrobenzene	3.547	2272430	142.445 ng/ml
6) T 3,5-Dinitroaniline	3.925	1667122	148.445 ug/L
7) T Nitrobenzene	4.788	1347763	138.552 ug/L
9) T 2,4,6-Trinitrotoluene	6.568f	1536761	151.061 ug/L
12) T 2,4-Dinitrotoluene	8.238f	2118214	142.003 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
Data File : HN006956.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 02-Nov-2014, 01:33
Operator : TP
Sample : F4325-03MS
Misc :
ALS Vial : 82 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
YS19-SB19-1014MS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 04:11:59 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Quant Title :
QLast Update : Sat Mar 07 03:03:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

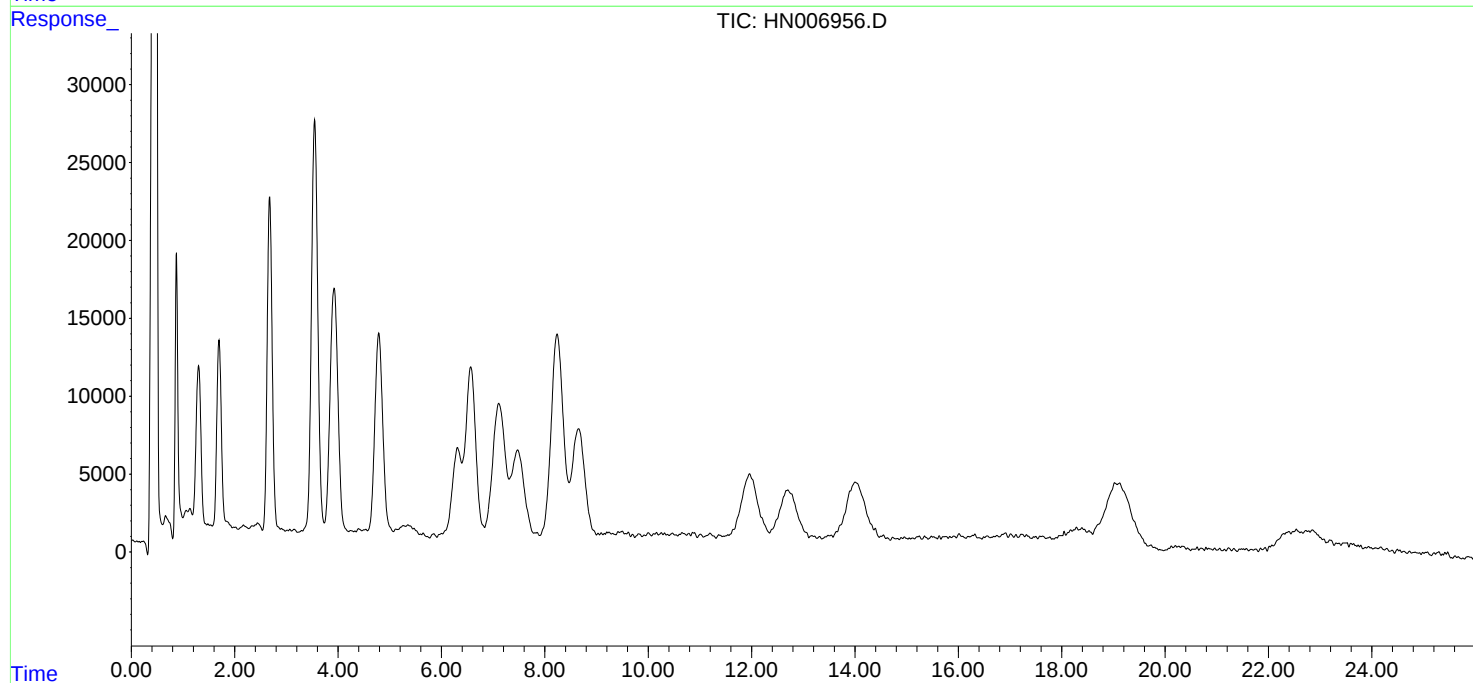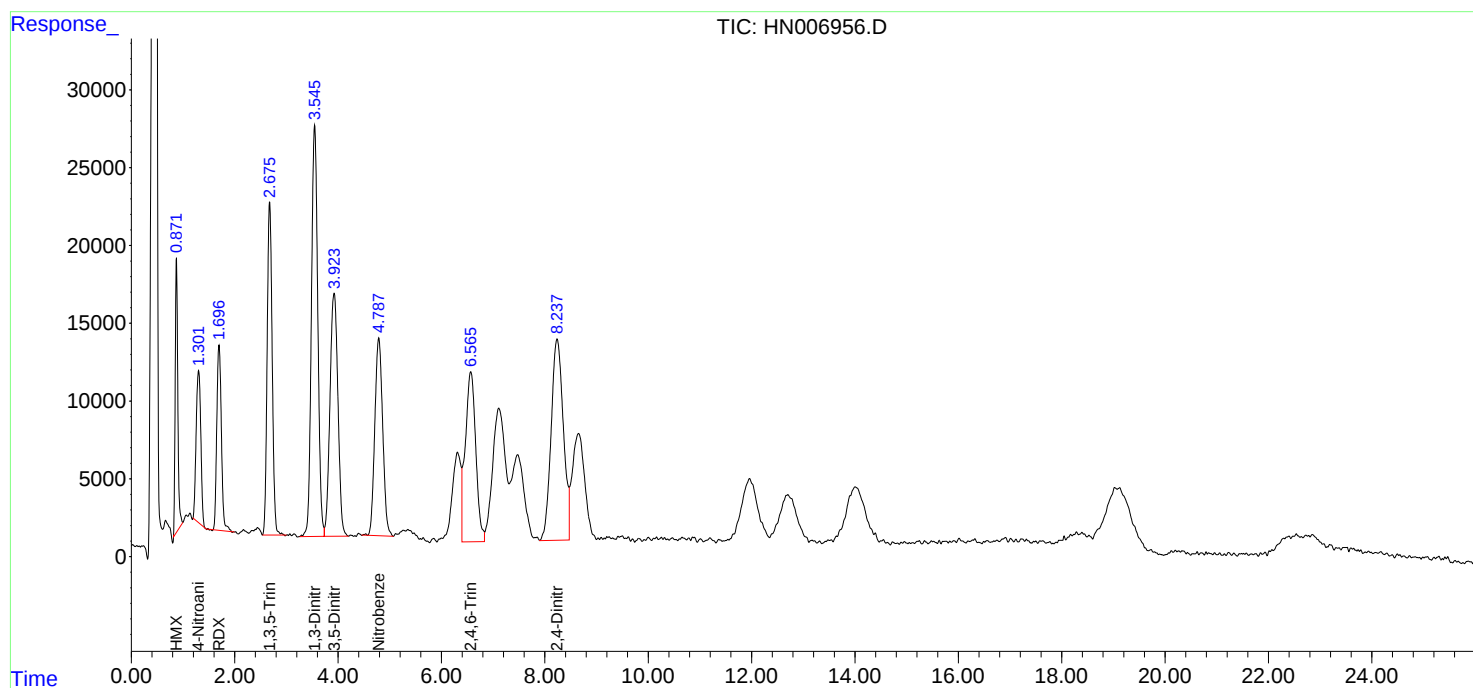


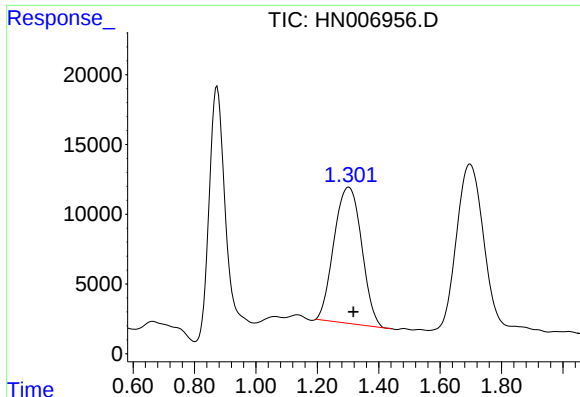

#1 4-Nitroaniline


R.T.: 1.302 min
Delta R.T.: -0.015 min
Response: 607948
Conc: 174.18 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-SB19-1014MS

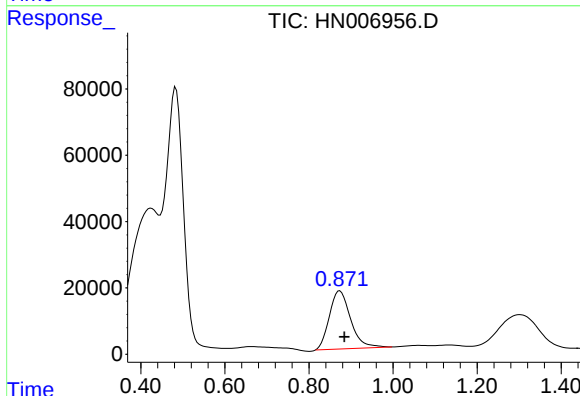


#2 HMX

R.T.: 0.874 min
Delta R.T.: -0.011 min
Response: 616690
Conc: 146.39 ug/L

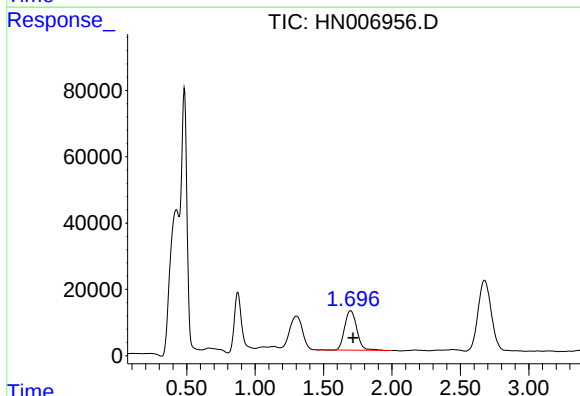


#3 RDX

R.T.: 1.698 min
Delta R.T.: -0.020 min
Response: 734804
Conc: 145.30 ug/L

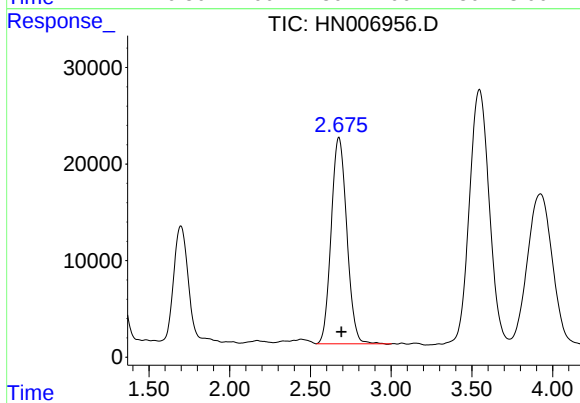

#4 1,3,5-Trinitrobenzene


R.T.: 2.677 min
Delta R.T.: -0.016 min
Response: 1434278
Conc: 140.78 ug/L

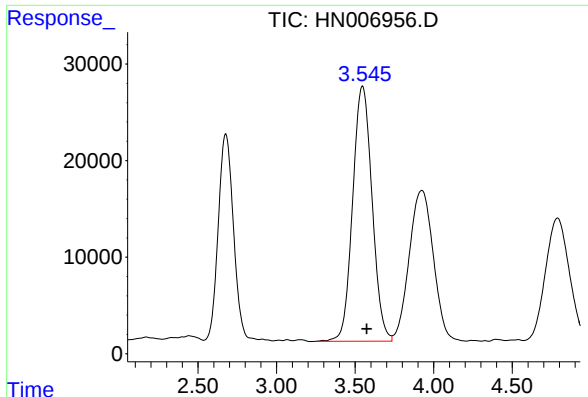

#5 1,3-Dinitrobenzene


R.T.: 3.547 min
Delta R.T.: -0.028 min
Response: 2272430
Conc: 142.45 ng/ml

Instrument :
HPLC_N
ClientSampleId :
YS19-SB19-1014MS

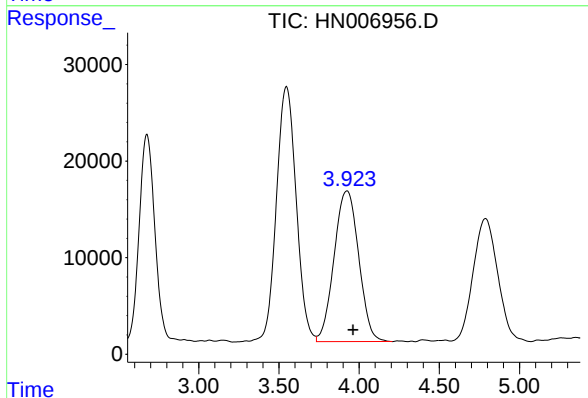


#6 3,5-Dinitroaniline

R.T.: 3.925 min
Delta R.T.: -0.037 min
Response: 1667122
Conc: 148.44 ug/L

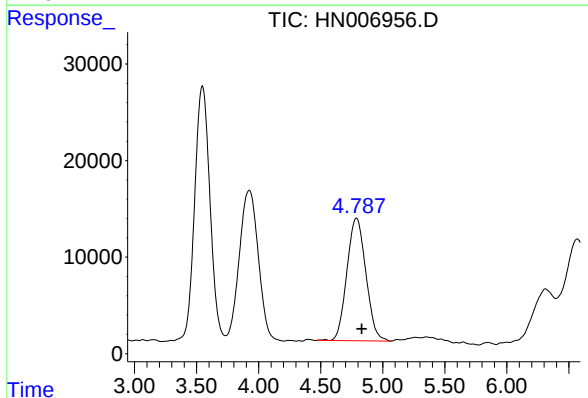


#7 Nitrobenzene

R.T.: 4.788 min
Delta R.T.: -0.042 min
Response: 1347763
Conc: 138.55 ug/L

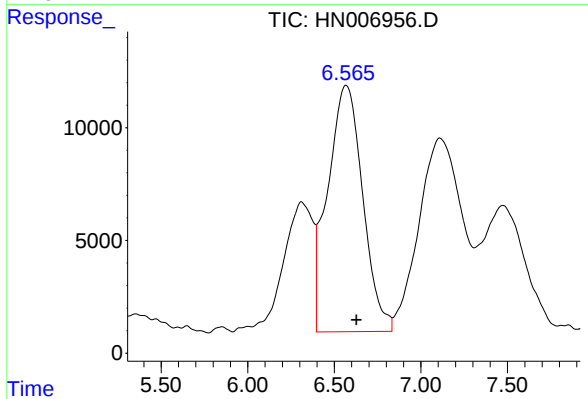

#9 2,4,6-Trinitrotoluene

R.T.: 6.568 min
Delta R.T.: -0.059 min
Response: 1536761
Conc: 151.06 ug/L

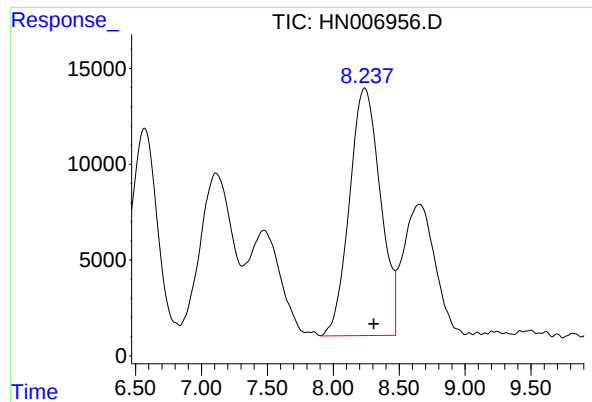

#12 2,4-Dinitrotoluene

R.T.: 8.238 min

Delta R.T.: -0.070 min

Response: 2118214

Conc: 142.00 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-SB19-1014MS