

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
 Data File : HN006958.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 02-Nov-2014, 02:29
 Operator : TP
 Sample : PB79844BS
 Misc :
 ALS Vial : 84 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 PB79844BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 04:12:25 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
 Quant Title :
 QLast Update : Sat Mar 07 03:03:02 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.296	637375	182.614 ug/L
Target Compounds			
2) T HMX	0.871	572236	135.842 ug/L
3) T RDX	1.679	664554	131.407 ug/L
4) T 1,3,5-Trinitrobenzene	2.659	1326369	130.193 ug/L
5) T 1,3-Dinitrobenzene	3.527	2072643	129.922 ng/ml
6) T 3,5-Dinitroaniline	3.901f	1496065	133.213 ug/L
7) T Nitrobenzene	4.767f	1233711	126.828 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
Data File : HN006958.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 02-Nov-2014, 02:29
Operator : TP
Sample : PB79844BS
Misc :
ALS Vial : 84 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
PB79844BS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 04:12:25 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Quant Title :
QLast Update : Sat Mar 07 03:03:02 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

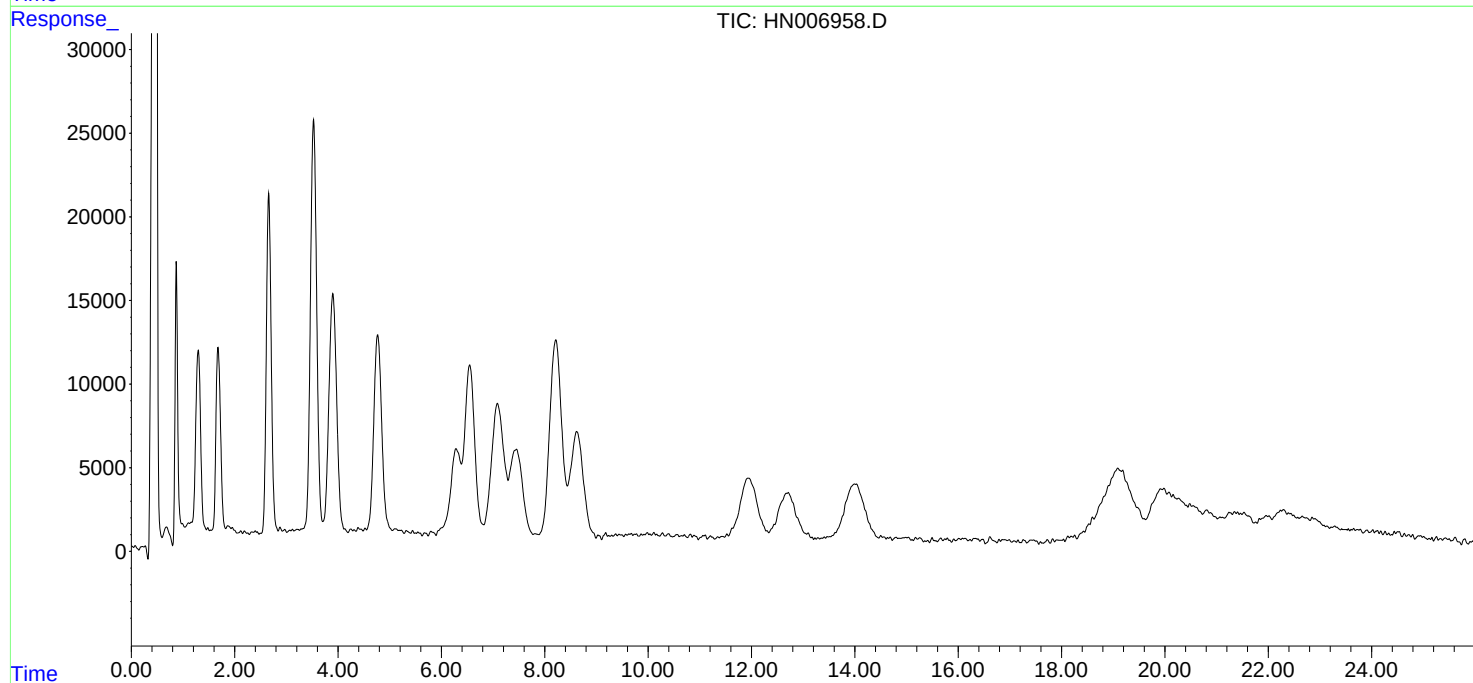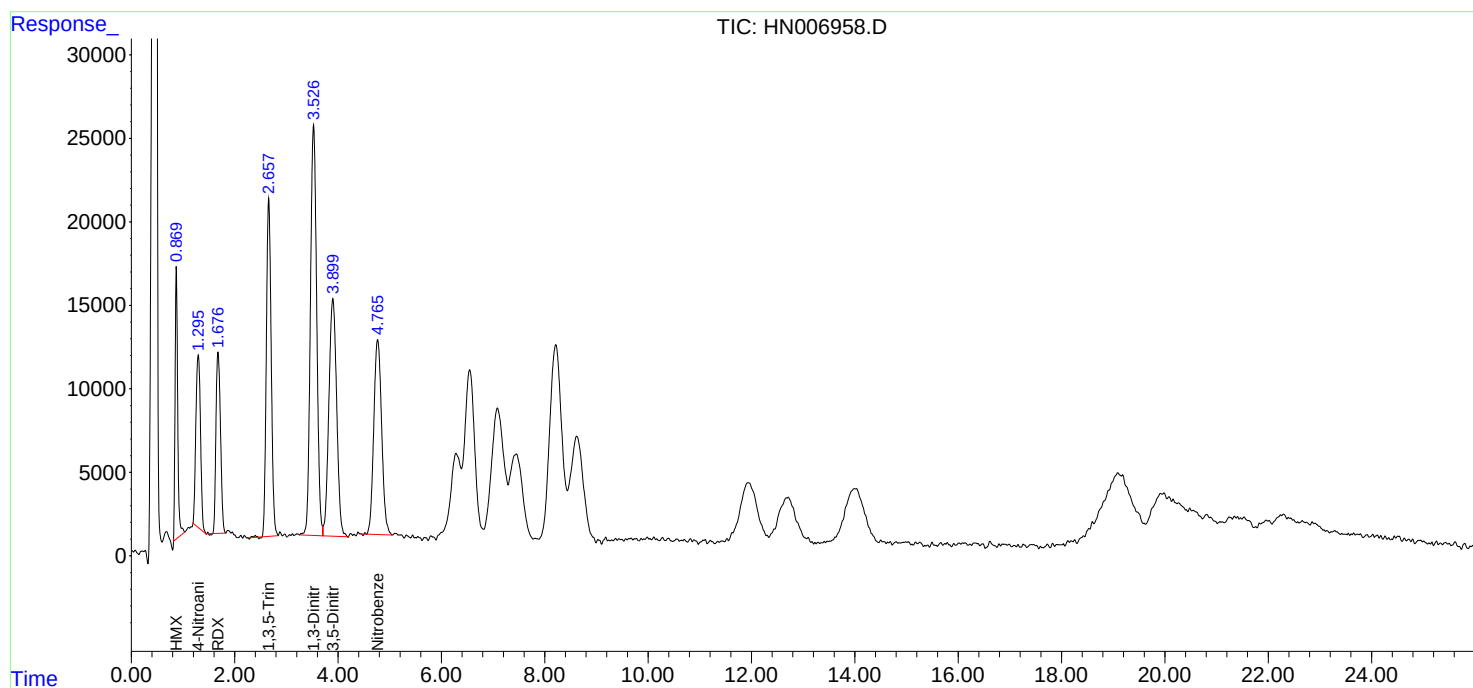


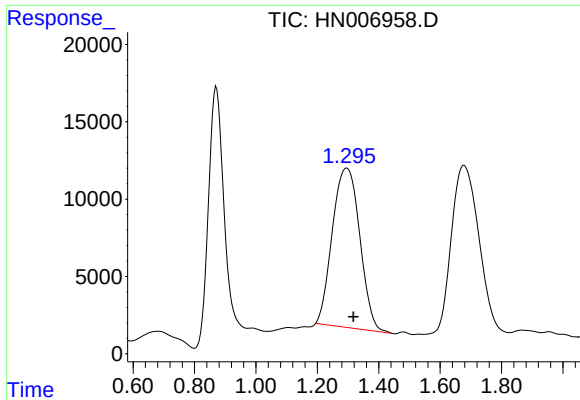

#1 4-Nitroaniline


R.T.: 1.296 min
Delta R.T.: -0.021 min
Response: 637375
Conc: 182.61 ug/L

Instrument :
HPLC_N
ClientSampleId :
PB79844BS

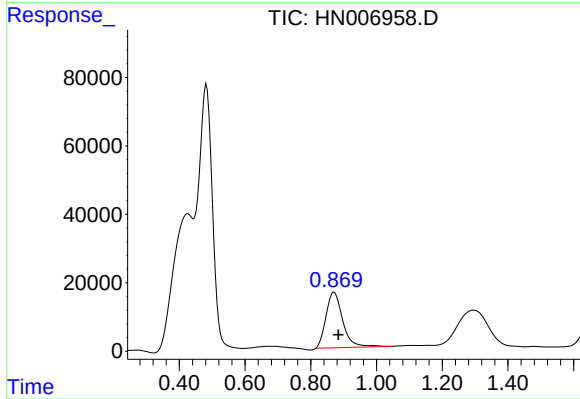


#2 HMX

R.T.: 0.871 min
Delta R.T.: -0.013 min
Response: 572236
Conc: 135.84 ug/L

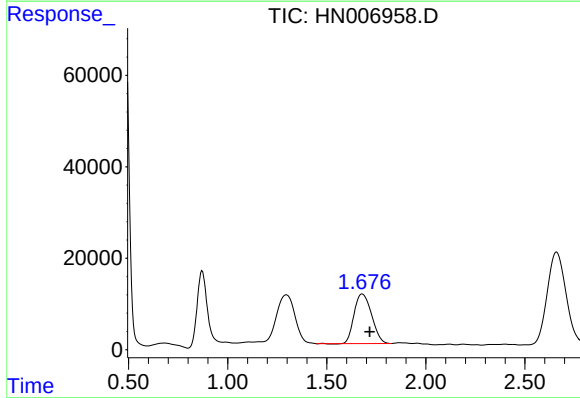


#3 RDX

R.T.: 1.679 min
Delta R.T.: -0.039 min
Response: 664554
Conc: 131.41 ug/L

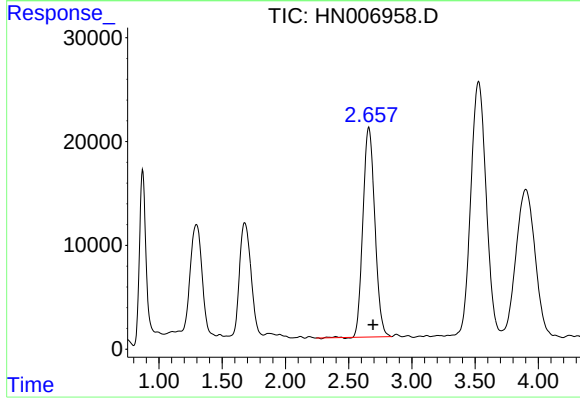

#4 1,3,5-Trinitrobenzene


R.T.: 2.659 min
Delta R.T.: -0.033 min
Response: 1326369
Conc: 130.19 ug/L

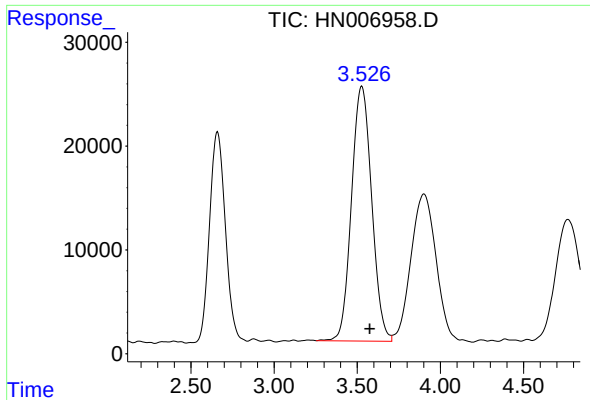

#5 1,3-Dinitrobenzene


R.T.: 3.527 min
Delta R.T.: -0.047 min
Response: 2072643
Conc: 129.92 ng/ml

Instrument :
HPLC_N
ClientSampleId :
PB79844BS

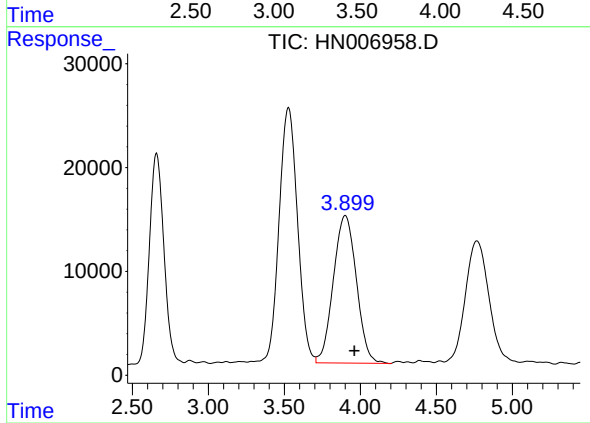

#6 3,5-Dinitroaniline

R.T.: 3.901 min
Delta R.T.: -0.061 min
Response: 1496065
Conc: 133.21 ug/L

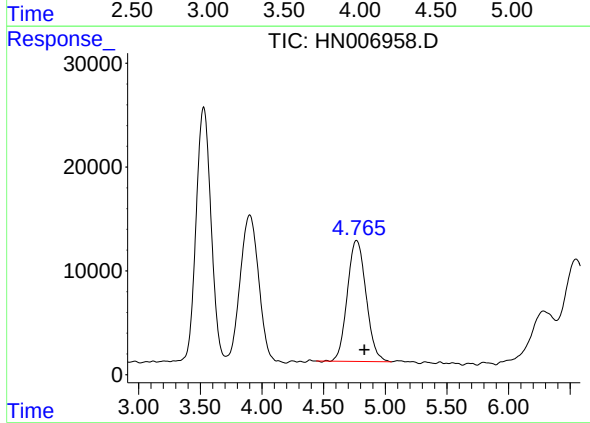

#7 Nitrobenzene

R.T.: 4.767 min
Delta R.T.: -0.064 min
Response: 1233711
Conc: 126.83 ug/L