

Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
 Data File : HN006914.D
 Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
 Acq On : 01-Nov-2014, 02:14
 Operator : TP
 Sample : F4372-06
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 HPLC_N
 ClientSampleId :
 YS19-SD16-1014

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 17:29:44 2015
 Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
 Quant Title :
 QLast Update : Fri Mar 06 17:29:40 2015
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.293	549660	157.482 ug/L
Target Compounds			
4) T 1,3,5-Trinitrobenzene	2.655	171146	16.799 ug/L
9) T 2,4,6-Trinitrotoluene	6.522	2318479	227.903 ug/L
10) T 2-Amino-4,6-dinitroto...	7.052	666779	60.535 ug/L
11) T 4-Amino-2,6-dinitroto...	7.413	1108277	195.068 ug/L

(f)=RT Delta > 1/2 Window



(m)=manual int.


Data Path : Z:\HPCHEM1\HPLC_N\Data\HN103114\
Data File : HN006914.D
Signal(s) : Signal #1: VWD1A.CH Signal #2: VWD1A.CH
Acq On : 01-Nov-2014, 02:14
Operator : TP
Sample : F4372-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
HPLC_N
ClientSampleId :
YS19-SD16-1014

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 17:29:44 2015
Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Quant Title :
QLast Update : Fri Mar 06 17:29:40 2015
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

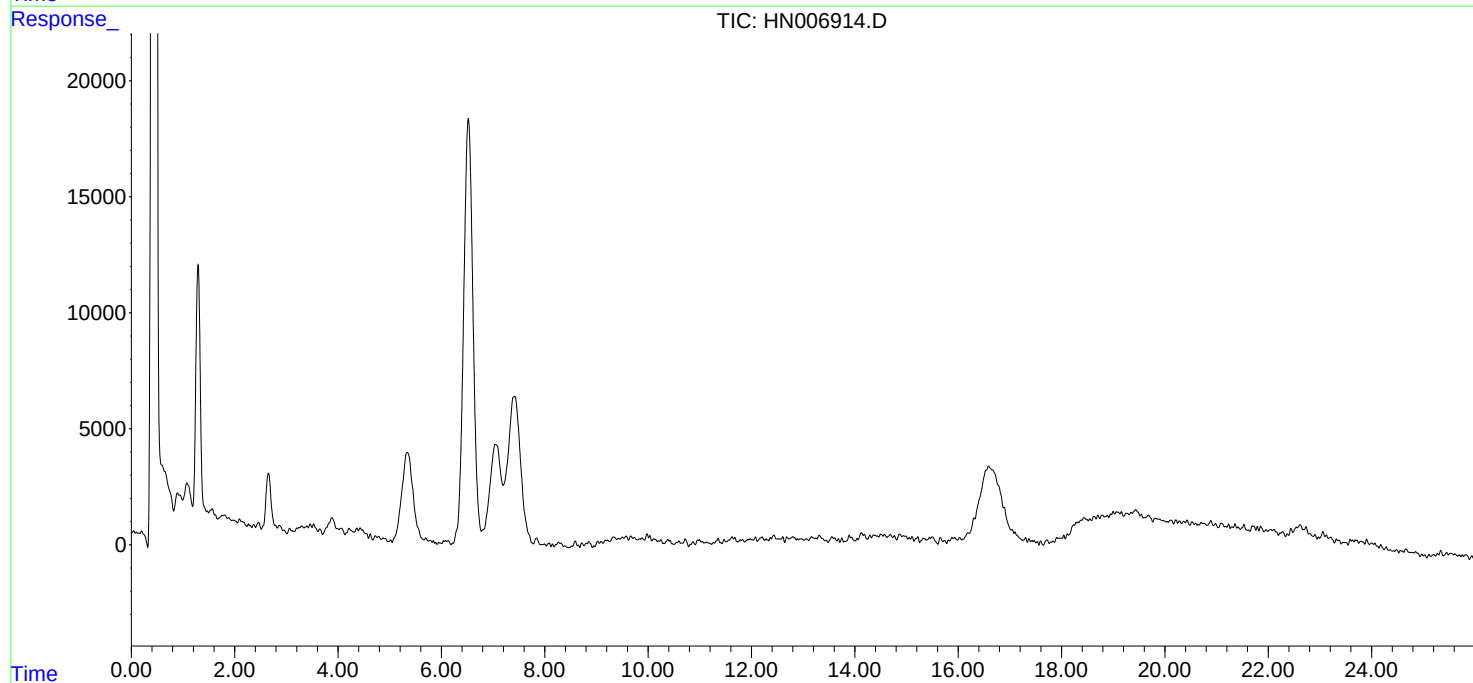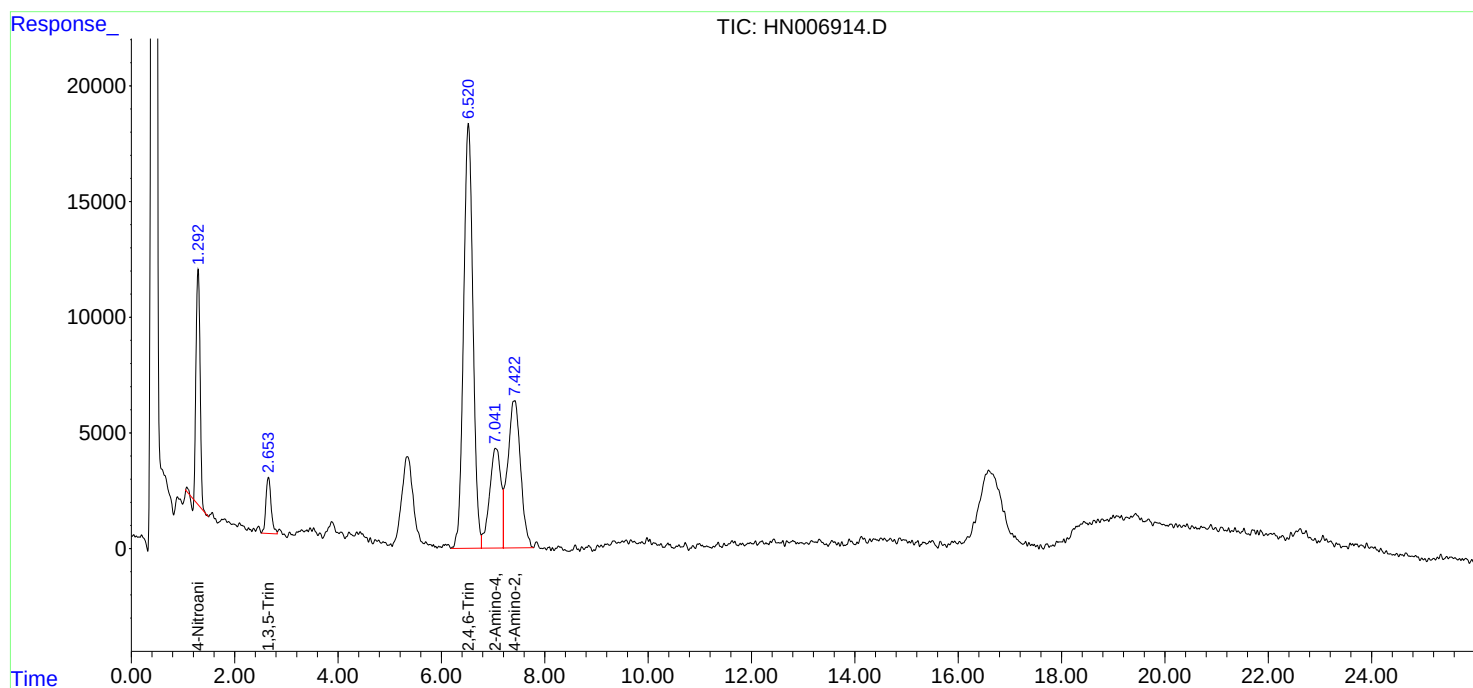


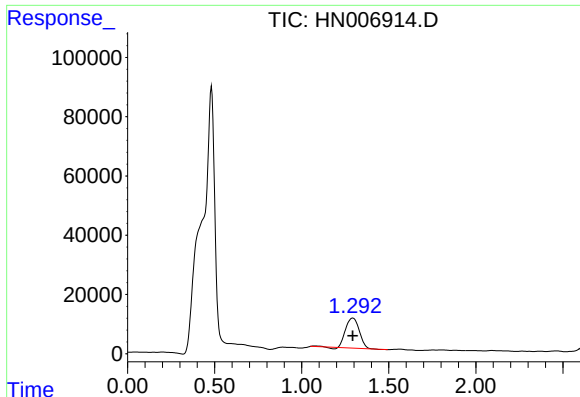

#1 4-Nitroaniline


R.T.: 1.293 min
Delta R.T.: 0.001 min
Response: 549660
Conc: 157.48 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-SD16-1014

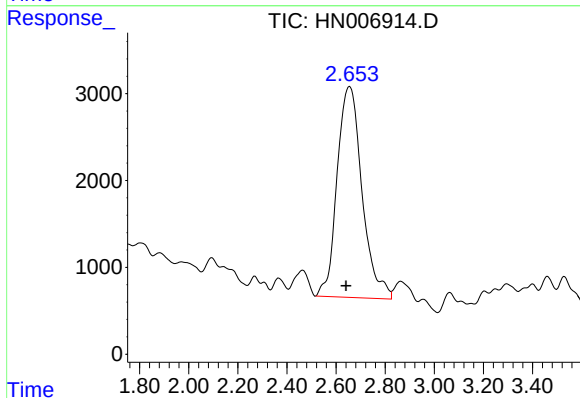


#4 1,3,5-Trinitrobenzene

R.T.: 2.655 min
Delta R.T.: 0.014 min
Response: 171146
Conc: 16.80 ug/L

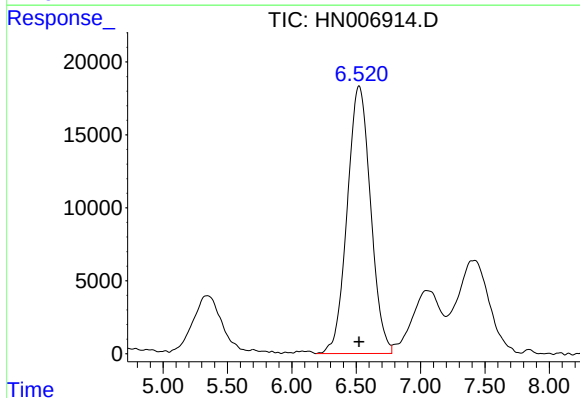


#9 2,4,6-Trinitrotoluene

R.T.: 6.522 min
Delta R.T.: 0.000 min
Response: 2318479
Conc: 227.90 ug/L

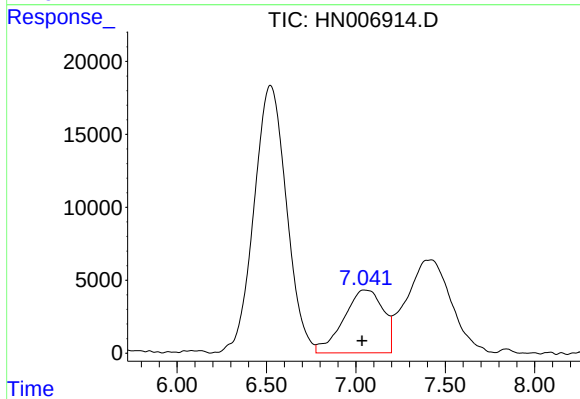

#10 2-Amino-4,6-dinitrotoluene

R.T.: 7.052 min
Delta R.T.: 0.017 min
Response: 666779
Conc: 60.53 ug/L

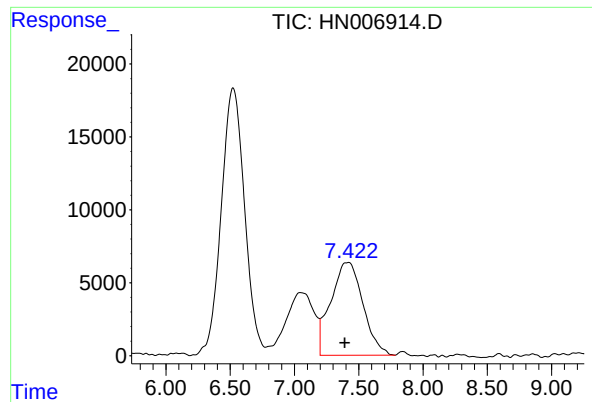

#11 4-Amino-2,6-dinitrotoluene

R.T.: 7.413 min
Delta R.T.: 0.022 min
Response: 1108277
Conc: 195.07 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-SD16-1014