

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN103114\HN006905.D\VWD1A.CH Vial: 25
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN103114\HN006905.D\VWD1A.CH
 Acq On : 31-Oct-2014, 22:02 Operator: TP
 Sample : F4379-18 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
 Quant Time: Nov 2 2:05 2014 Quant Results File: HN103114.RES

Instrument :
 HPLC_N
 ClientSampleId :
 YS19-EB01-102014-SO

Manual Integrations
 APPROVED

ugo
 11/14/2014 10:32:35 AM

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
 Title :
 Last Update : Sat Nov 01 07:07:53 2014
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.29	1143130	314.457 ug/L m
Target Compounds			
6) T 3,5-Dinitroaniline	4.05	543436	48.460 ug/L m

 Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN006905.D HN103114.M Sat Nov 08 04:38:20 2014

Quantitation Report

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN103114\HN006905.D\VWD1A.CH Vial: 25
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN103114\HN006905.D\VWD1A.CH
 Acq On : 31-Oct-2014, 22:02 Operator: TP
 Sample : F4379-18 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
 Quant Time: Nov 2 2:05 2014 Quant Results File: HN103114.RES



Instrument :
 HPLC_N
 ClientSampleId :
 YS19-EB01-102014-SO


Manual Integrations
 APPROVED

ugo
 11/14/2014 10:32:35 AM

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
 Title :
 Last Update : Sat Nov 01 07:07:53 2014
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

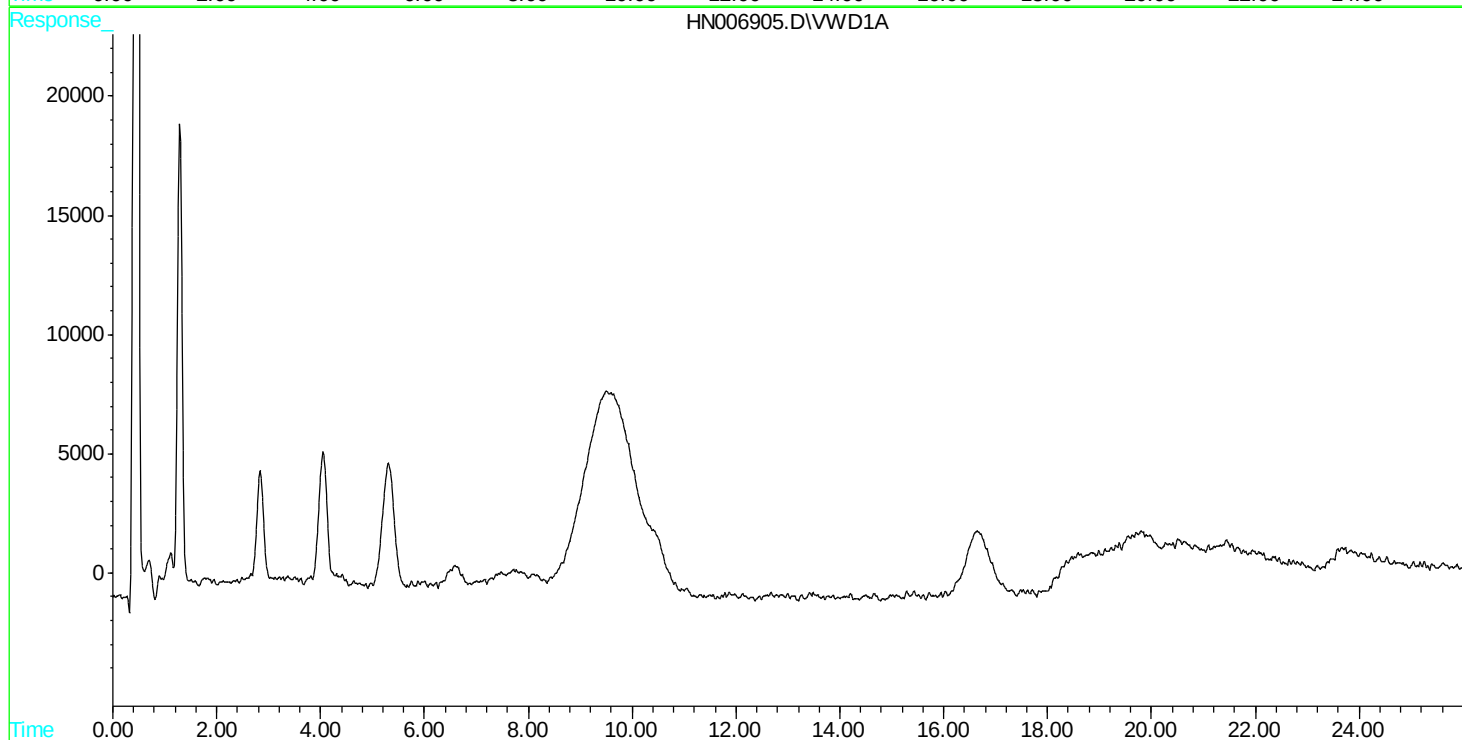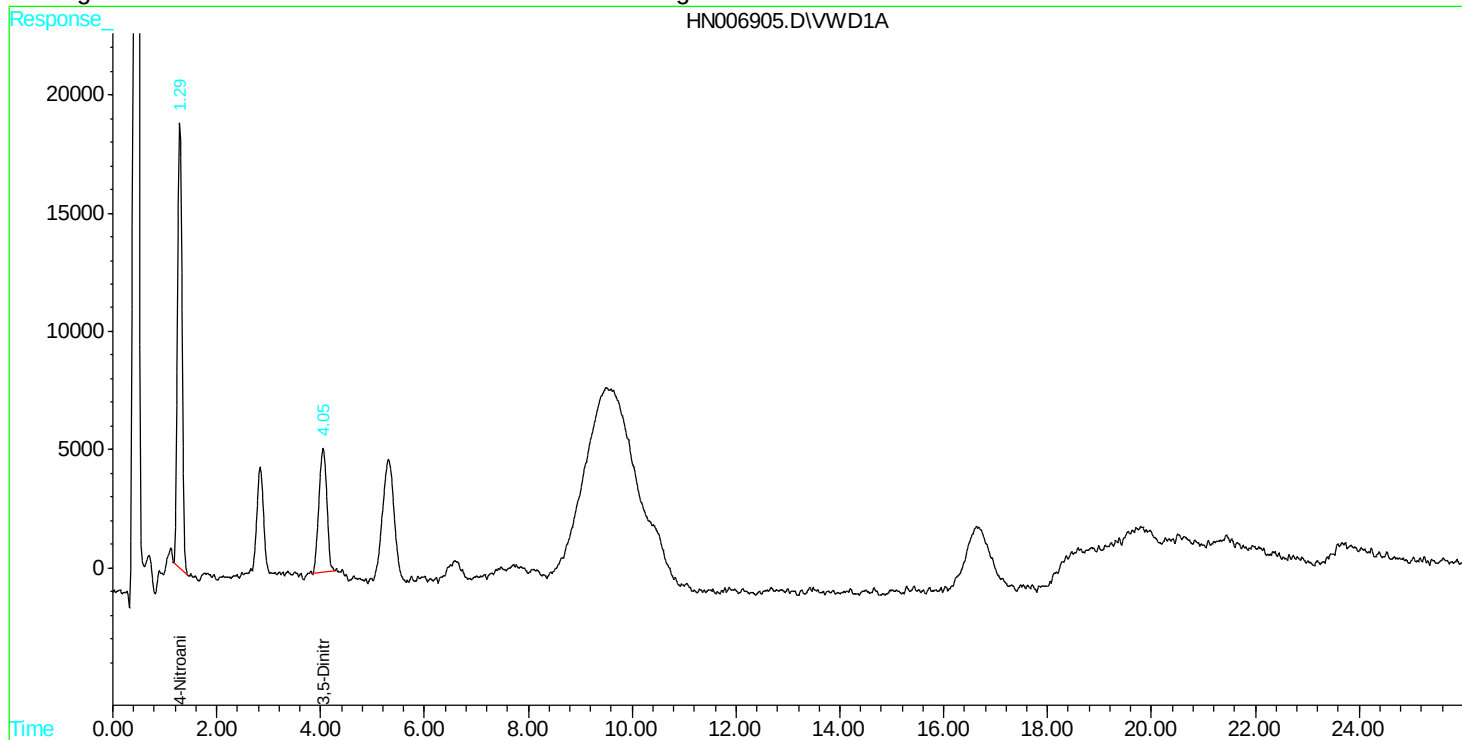

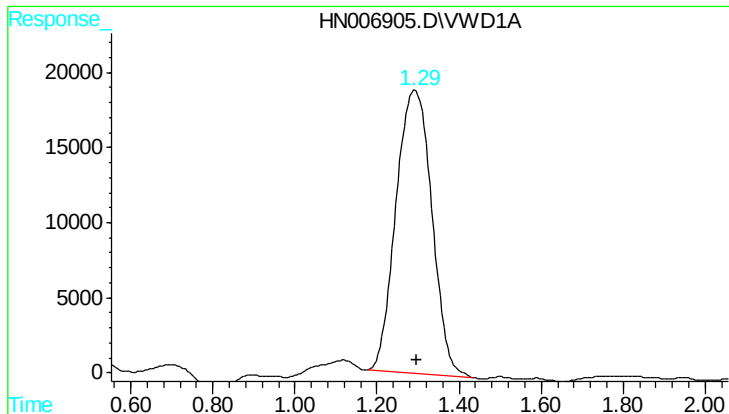


#1 4-Nitroaniline

R.T.: 1.291 min
 Delta R.T.: -0.005 min
 Response: 1143130
 Conc: 314.46 ug/L m

Instrument :
 HPLC_N
 ClientSampleId :
 YS19-EB01-102014-SO

Manual Integrations
 APPROVED

ugo
 11/14/2014 10:32:35 AM

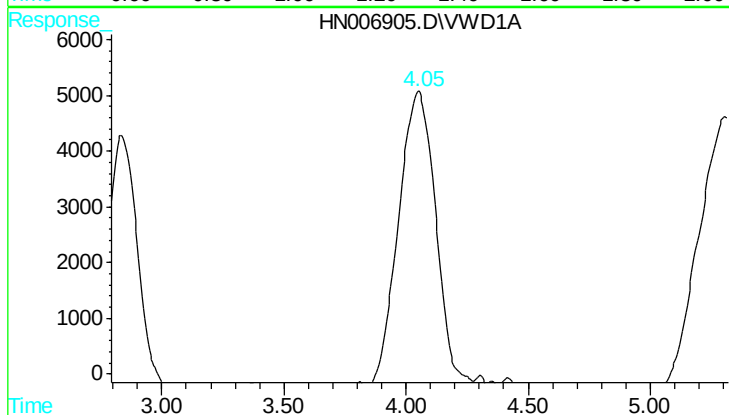

#6 3,5-Dinitroaniline

R.T.: 4.049 min
 Delta R.T.: 0.176 min
 Response: 543436
 Conc: 48.46 ug/L m