

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN103114\HN006909.D\VWD1A.CH Vial: 29
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN103114\HN006909.D\VWD1A.CH
 Acq On : 31-Oct-2014, 23:54 Operator: TP
 Sample : F4372-02MS Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
 Quant Time: Nov 2 2:11 2014 Quant Results File: HN103114.RES

Instrument :
 HPLC_N
 ClientSampleId :
 YS19-SD01-1014MS

Manual Integrations
 APPROVED

ugo
 11/14/2014 10:32:55 AM

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
 Title :
 Last Update : Sat Nov 01 07:07:53 2014
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.30	523813	144.093 ug/L m
Target Compounds			
9) T 2,4,6-Trinitrotoluene	6.54	431228	42.527 ug/L m

 Analyst Signature: _____ Analyst Name: _____ Date: _____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #: _____

___Peak Integrated by software incorrectly.Compound #: _____

___OTHER: _____ Compound #: _____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN006909.D HN103114.M Sat Nov 08 04:39:11 2014

Quantitation Report

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN103114\HN006909.D\VWD1A.CH Vial: 29
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN103114\HN006909.D\VWD1A.CH
 Acq On : 31-Oct-2014, 23:54 Operator: TP
 Sample : F4372-02MS Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
 Quant Time: Nov 2 2:11 2014 Quant Results File: HN103114.RES



Instrument :
 HPLC_N
 ClientSampleId :
 YS19-SD01-1014MS


Manual Integrations
 APPROVED

ugo
 11/14/2014 10:32:55 AM

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
 Title :
 Last Update : Sat Nov 01 07:07:53 2014
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

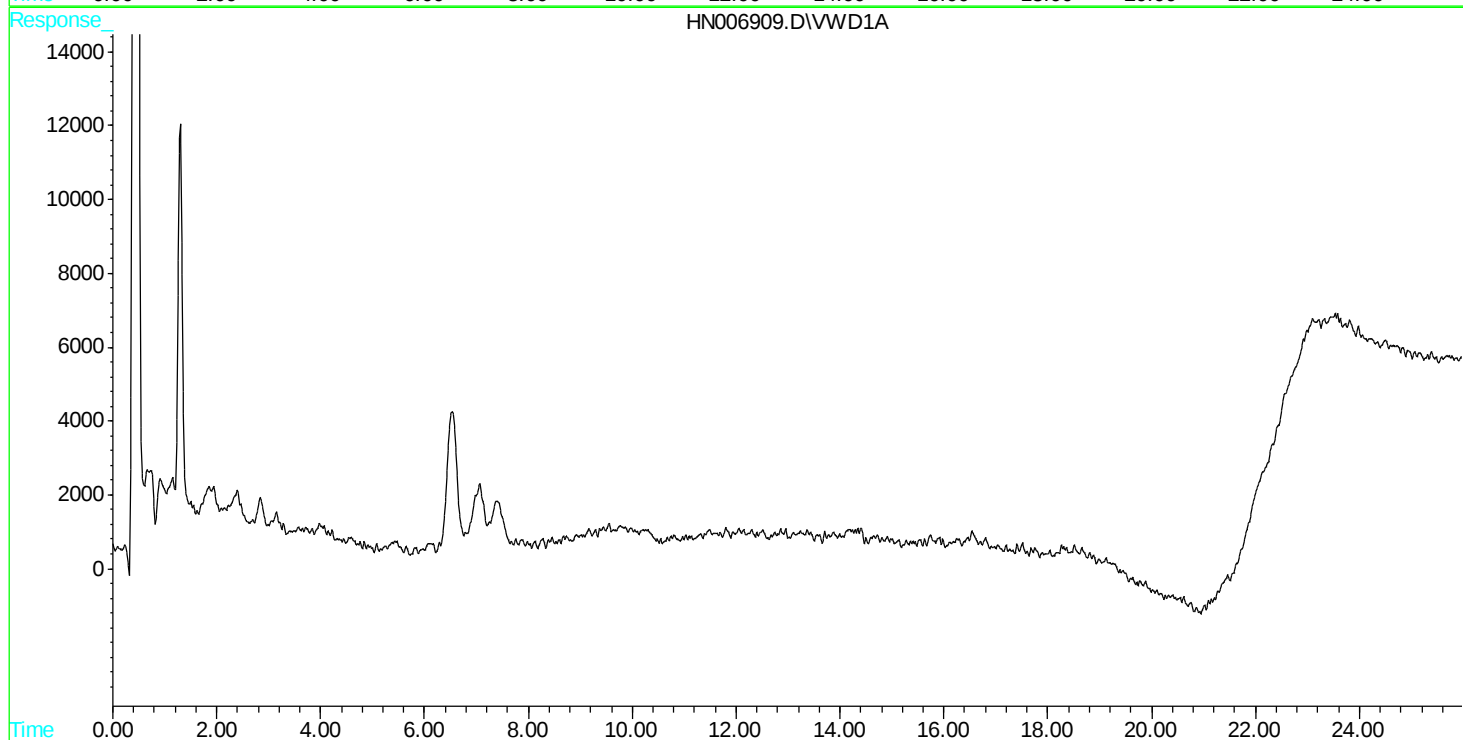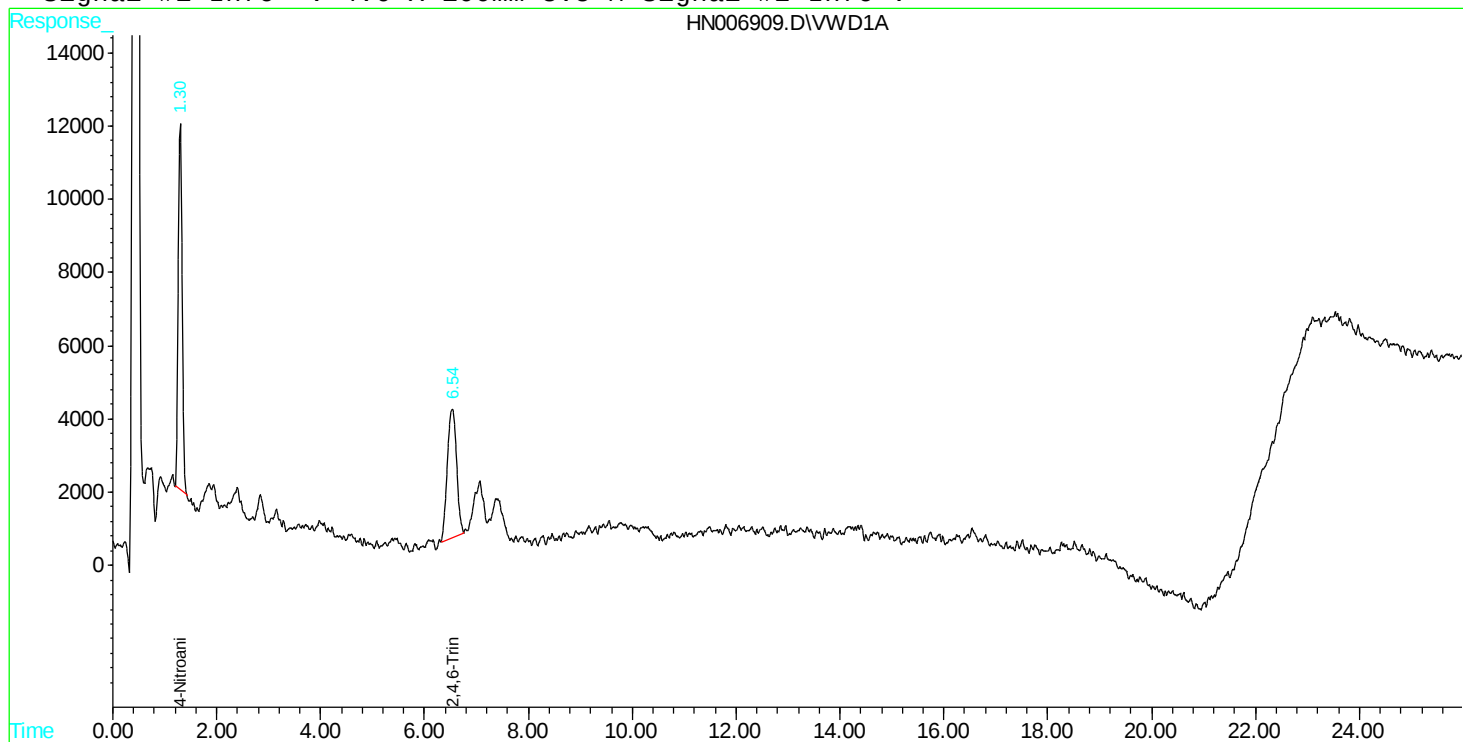

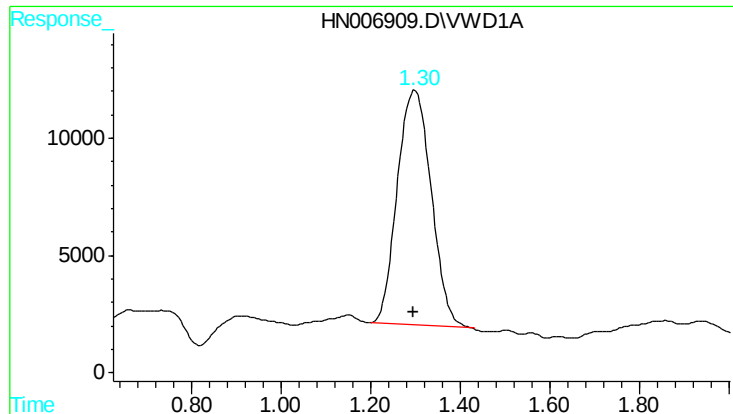


#1 4-Nitroaniline

R.T.: 1.297 min
Delta R.T.: 0.000 min
Response: 523813
Conc: 144.09 ug/L m

Instrument :
HPLC_N
ClientSampleId :
YS19-SD01-1014MS

Manual Integrations
APPROVED

ugo
11/14/2014 10:32:55 AM

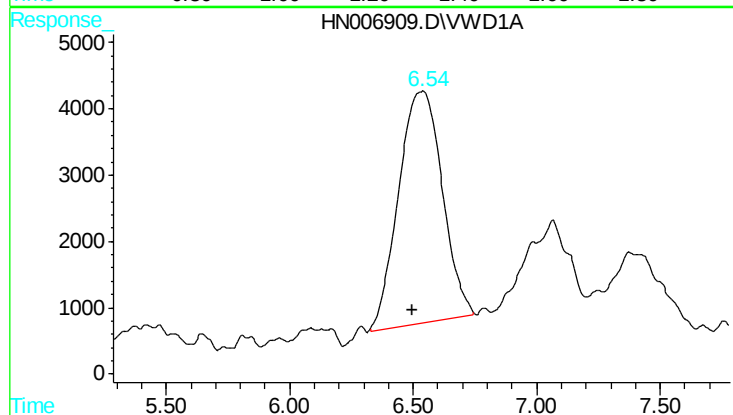

#9 2,4,6-Trinitrotoluene

R.T.: 6.538 min
Delta R.T.: 0.042 min
Response: 431228
Conc: 42.53 ug/L m