

Signal #1 : Z:\HPCHEM1\HPLC\_N\DATA\HN103114\HN006920.D\VWD1A.CH Vial: 39  
 Signal #2 : Z:\HPCHEM1\HPLC\_N\DATA\HN103114\HN006920.D\VWD1A.CH  
 Acq On : 01-Nov-2014, 05:03 Operator: TP  
 Sample : F4372-14 Inst : G1314A  
 Misc : Multiplr: 1.00  
 IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e  
 Quant Time: Nov 2 2:34 2014 Quant Results File: HN103114.RES

Instrument :  
 HPLC\_N  
 ClientSampleId :  
 YS19-SD14-1014

Manual Integrations  
 APPROVED

ugo  
 11/14/2014 10:33:45 AM

Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN103114.M  
 Title :  
 Last Update : Sat Nov 01 07:07:53 2014  
 Response via : Initial Calibration  
 DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul  
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

| Compound                    | R.T. | Response | Conc Units     |
|-----------------------------|------|----------|----------------|
| -----                       |      |          |                |
| System Monitoring Compounds |      |          |                |
| 1) S 4-Nitroaniline         | 1.30 | 546310   | 150.281 ug/L m |

Target Compounds

-----  
 Analyst Signature:\_\_\_\_\_ Analyst Name:\_\_\_\_\_ Date:\_\_\_\_\_

-----REASONS FOR MANUAL INTEGRATIONS-----

\_\_\_Poor resolution of peaks exhibited on chromatogram.Compound #:\_\_\_\_\_

\_\_\_Peak Integrated by software incorrectly.Compound #:\_\_\_\_\_

\_\_\_OTHER:\_\_\_\_\_Compound #:\_\_\_\_\_

(f)=RT Delta > 1/2 Window (m)=manual int.

HN006920.D HN103114.M Sat Nov 08 04:41:55 2014

# Quantitation Report

Signal #1 : Z:\HPCHEM1\HPLC\_N\DATA\HN103114\HN006920.D\VWD1A.CH Vial: 39  
 Signal #2 : Z:\HPCHEM1\HPLC\_N\DATA\HN103114\HN006920.D\VWD1A.CH  
 Acq On : 01-Nov-2014, 05:03 Operator: TP  
 Sample : F4372-14 Inst : G1314A  
 Misc : Multiplr: 1.00  
 IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e  
 Quant Time: Nov 2 2:34 2014 Quant Results File: HN103114.RES



Instrument :  
 HPLC\_N  
 ClientSampleId :  
 YS19-SD14-1014


Manual Integrations  
 APPROVED

ugo  
 11/14/2014 10:33:45 AM

Quant Method : Z:\HPCHEM1\HPLC\_N\METHODS\HN103114.M  
 Title :  
 Last Update : Sat Nov 01 07:07:53 2014  
 Response via : Multiple Level Calibration  
 DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul  
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:  
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

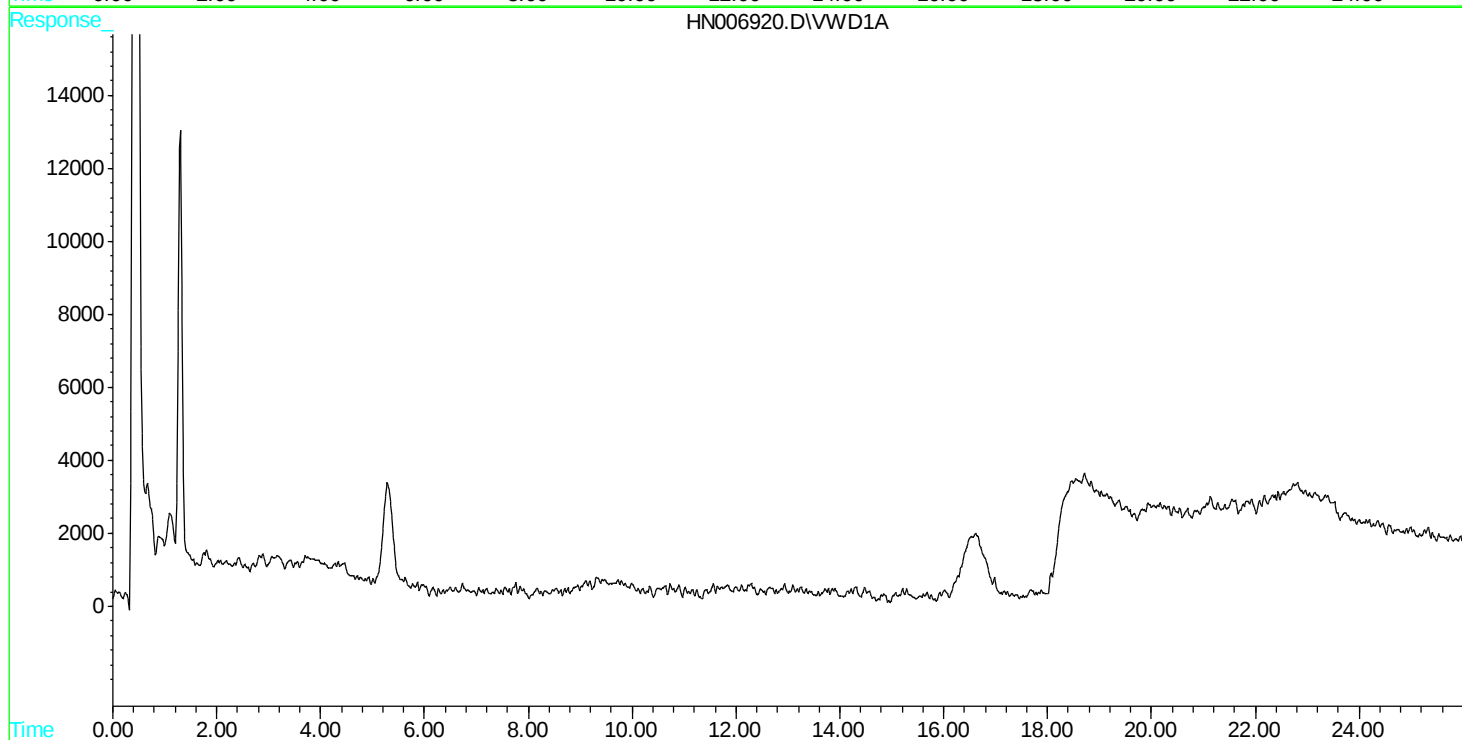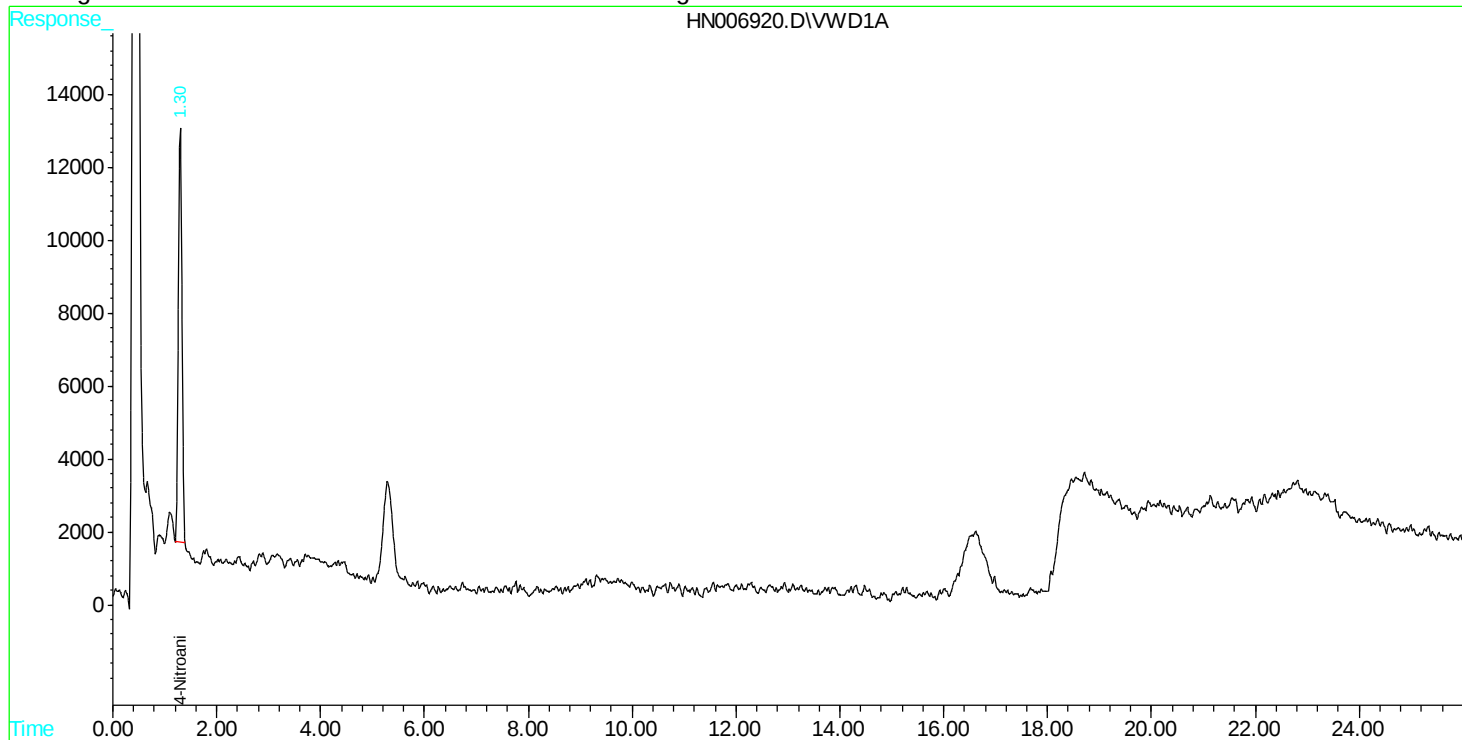

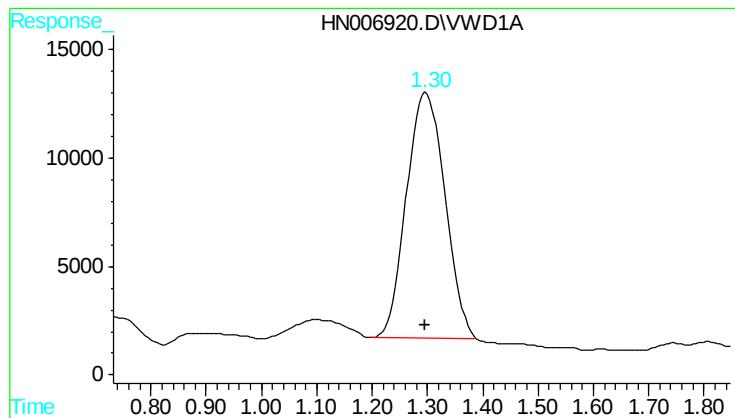

#1 4-Nitroaniline

R.T.: 1.296 min  
Delta R.T.: 0.000 min  
Response: 546310  
Conc: 150.28 ug/L m

Instrument :  
HPLC\_N  
ClientSampleId :  
YS19-SD14-1014

Manual Integrations  
APPROVED

ugo  
11/14/2014 10:33:45 AM