

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN103114\HN006939.D\VWD1A.CH Vial: 56
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN103114\HN006939.D\VWD1A.CH
 Acq On : 01-Nov-2014, 17:37 Operator: TP
 Sample : F4379-09 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
 Quant Time: Nov 2 3:52 2014 Quant Results File: HN103114.RES

Instrument :
 HPLC_N
 ClientSampleId :
 YS19-SS35-1014

Manual Integrations
 APPROVED

ugo
 11/14/2014 10:35:23 AM

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
 Title :
 Last Update : Sat Nov 01 07:07:53 2014
 Response via : Initial Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.30	569912	156.774 ug/L m

Target Compounds

 Analyst Signature: _____ Analyst Name: _____ Date: _____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #: _____

___Peak Integrated by software incorrectly.Compound #: _____

___OTHER: _____ Compound #: _____

(f)=RT Delta > 1/2 Window (m)=manual int.

HN006939.D HN103114.M Sat Nov 08 04:46:58 2014

Quantitation Report

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN103114\HN006939.D\VWD1A.CH Vial: 56
 Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN103114\HN006939.D\VWD1A.CH
 Acq On : 01-Nov-2014, 17:37 Operator: TP
 Sample : F4379-09 Inst : G1314A
 Misc : Multiplr: 1.00
 IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
 Quant Time: Nov 2 3:52 2014 Quant Results File: HN103114.RES



Instrument :
 HPLC_N
 ClientSampleId :
 YS19-SS35-1014


Manual Integrations
 APPROVED

ugo
 11/14/2014 10:35:23 AM

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
 Title :
 Last Update : Sat Nov 01 07:07:53 2014
 Response via : Multiple Level Calibration
 DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
 Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
 Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

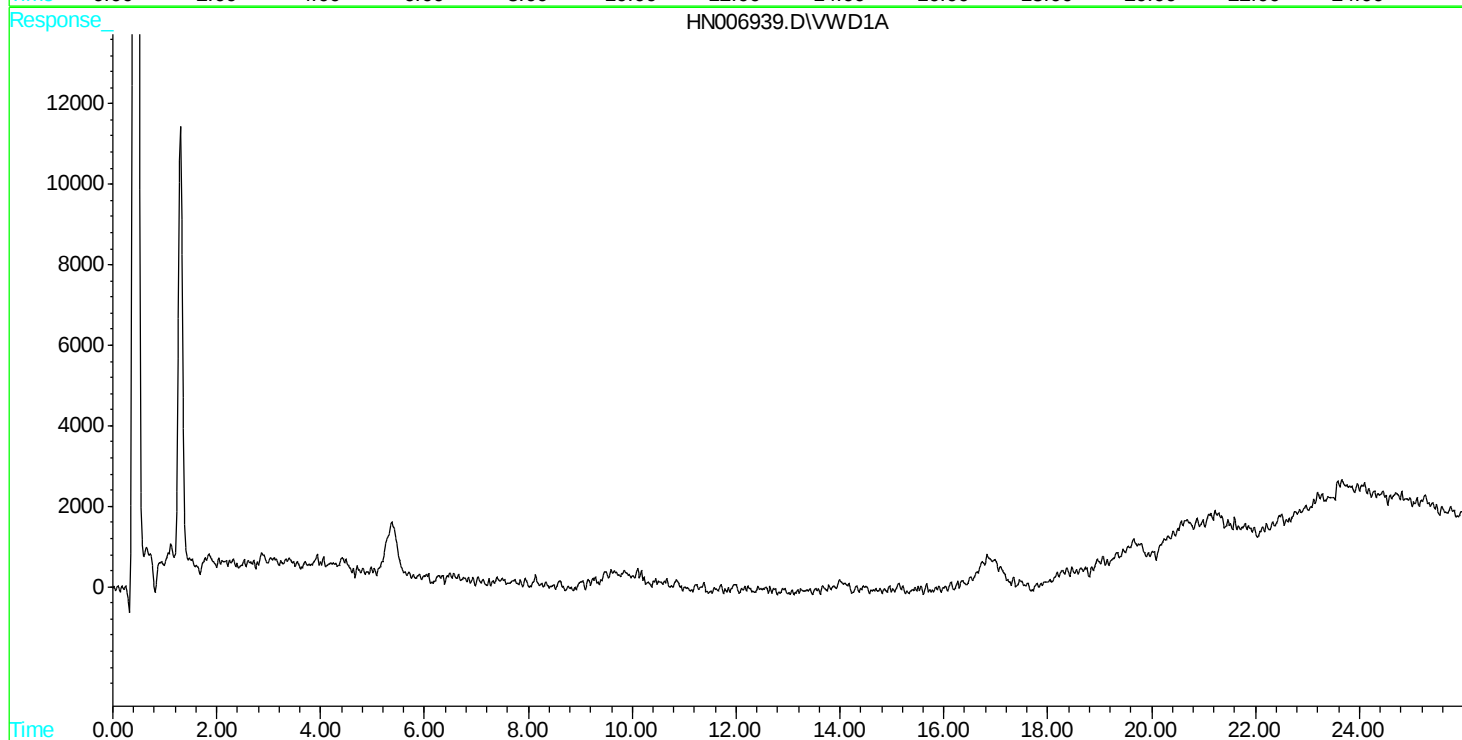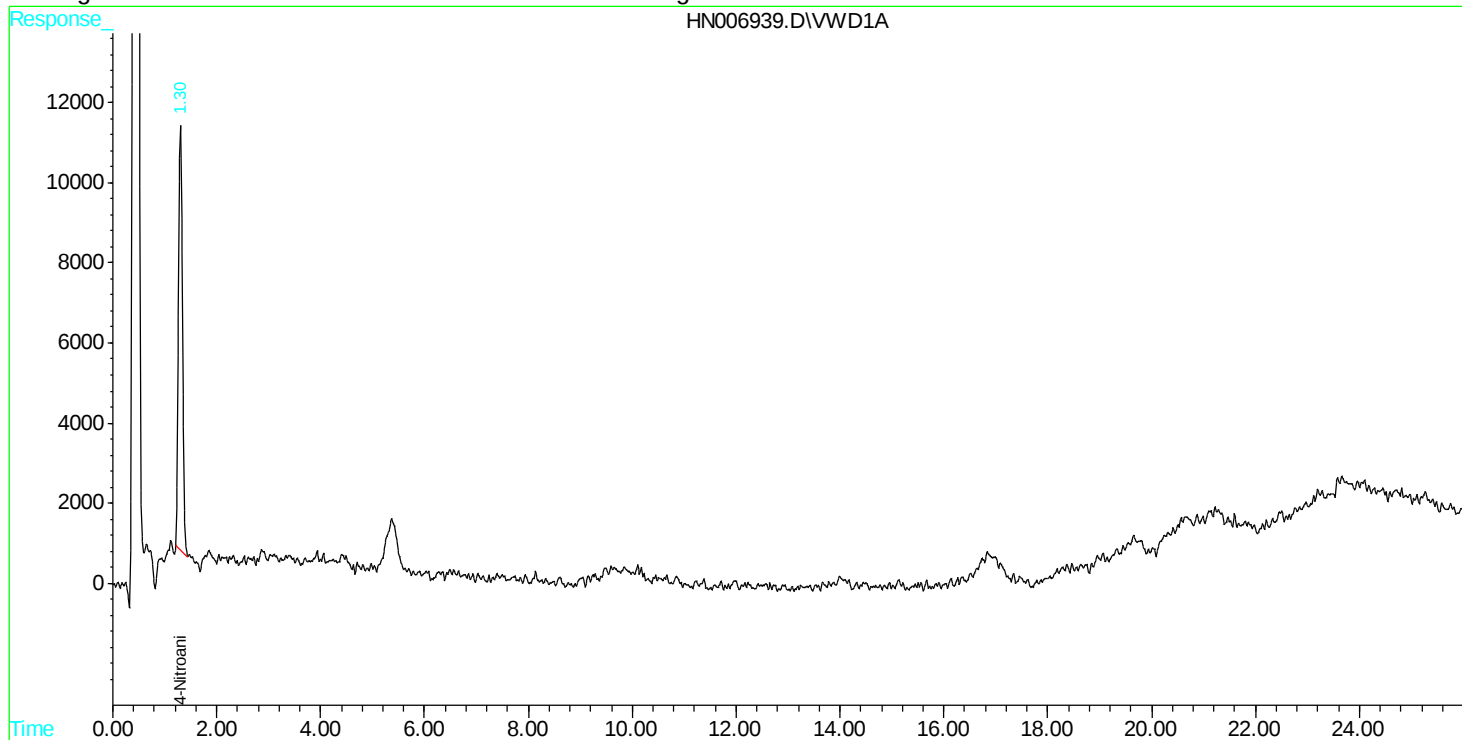

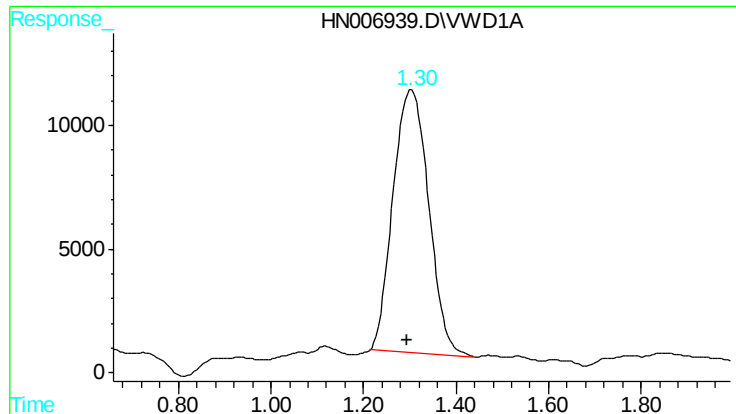

#1 4-Nitroaniline

R.T.: 1.302 min
Delta R.T.: 0.006 min
Response: 569912
Conc: 156.77 ug/L m

Instrument :
HPLC_N
ClientSampleId :
YS19-SS35-1014

Manual Integrations
APPROVED

ugo
11/14/2014 10:35:23 AM