

Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN103114\HN006955.D\VWD1A.CH Vial: 81
Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN103114\HN006955.D\VWD1A.CH
Acq On : 02-Nov-2014, 01:05 Operator: TP
Sample : F4325-02 Inst : G1314A
Misc : Multiplr: 1.00
IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
Quant Time: Nov 2 4:24 2014 Quant Results File: HN103114.RES

Instrument :
HPLC_N
ClientSampleId :
YS19-SB19-1014

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Title :
Last Update : Sat Nov 01 07:07:53 2014
Response via : Initial Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
1) S 4-Nitroaniline	1.30	19395744	5335.457 ug/L
Target Compounds			

Analyst Signature:_____ Analyst Name:_____ Date:_____

-----REASONS FOR MANUAL INTEGRATIONS-----

___Poor resolution of peaks exhibited on chromatogram.Compound #:_____

___Peak Integrated by software incorrectly.Compound #:_____

___OTHER:_____Compound #:_____

(f)=RT Delta > 1/2 Window (m)=manual int.



HN006955.D HN103114.M Sat Nov 08 04:52:23 2014


Signal #1 : Z:\HPCHEM1\HPLC_N\DATA\HN103114\HN006955.D\VWD1A.CH Vial: 81
Signal #2 : Z:\HPCHEM1\HPLC_N\DATA\HN103114\HN006955.D\VWD1A.CH
Acq On : 02-Nov-2014, 01:05 Operator: TP
Sample : F4325-02 Inst : G1314A
Misc : Multiplr: 1.00
IntFile Signal #1: autoint1.e IntFile Signal #2: autoint2.e
Quant Time: Nov 2 4:24 2014 Quant Results File: HN103114.RES

Instrument :
HPLC_N
ClientSampleId :
YS19-SB19-1014

Quant Method : Z:\HPCHEM1\HPLC_N\METHODS\HN103114.M
Title :
Last Update : Sat Nov 01 07:07:53 2014
Response via : Multiple Level Calibration
DataAcq Meth : 8330AGIP.M

Volume Inj. : 50 ul
Signal #1 Phase : ZORBAX Extend-C18 Signal #2 Phase:
Signal #1 Info : 4.6 X 100mm 3.5-M Signal #2 Info :

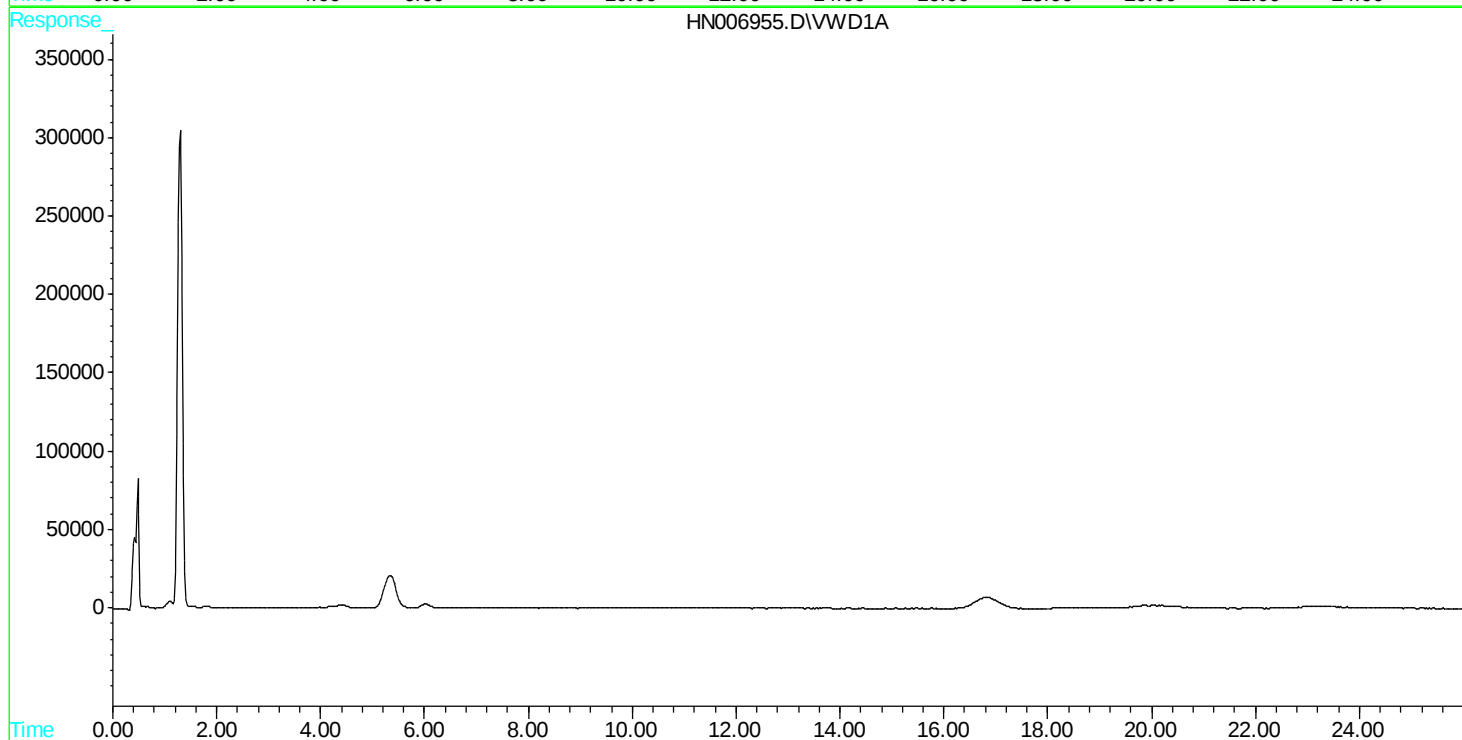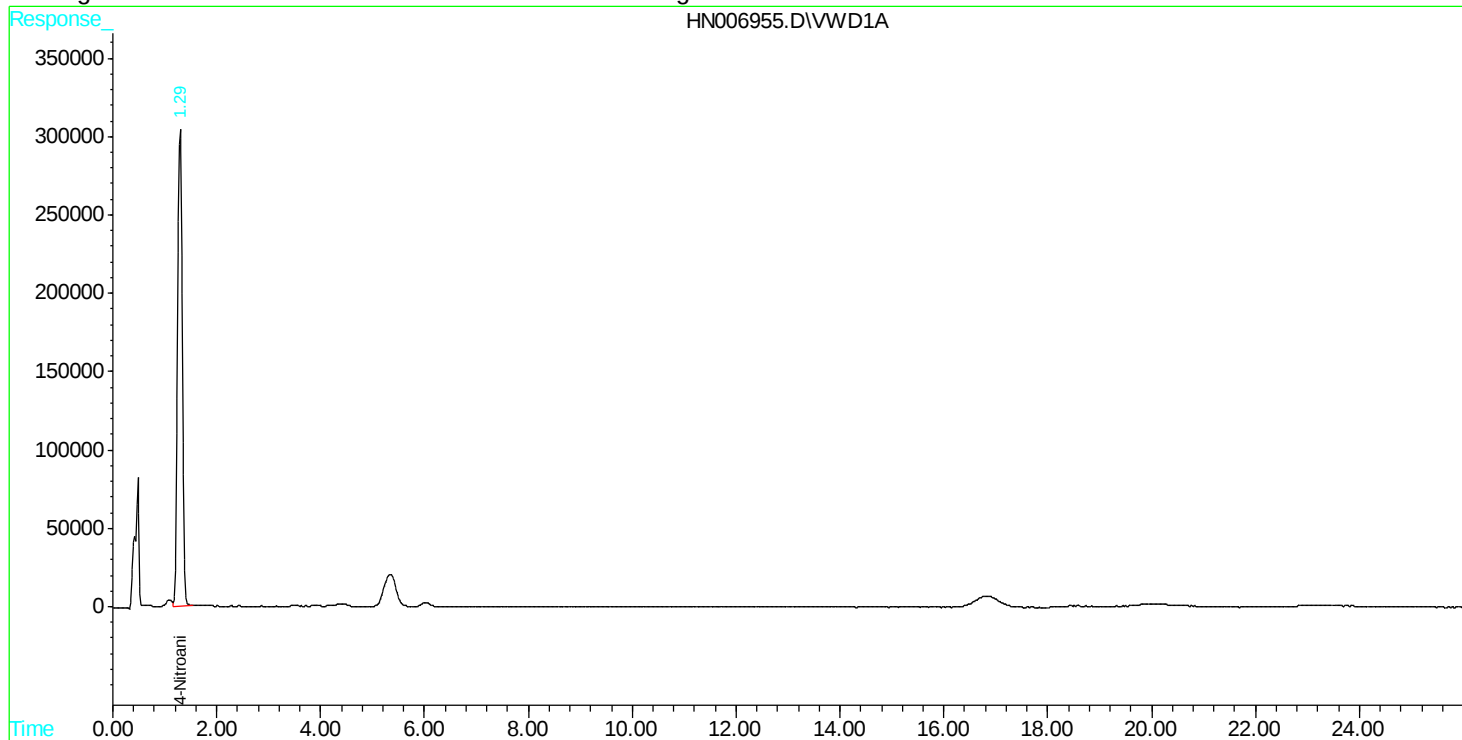

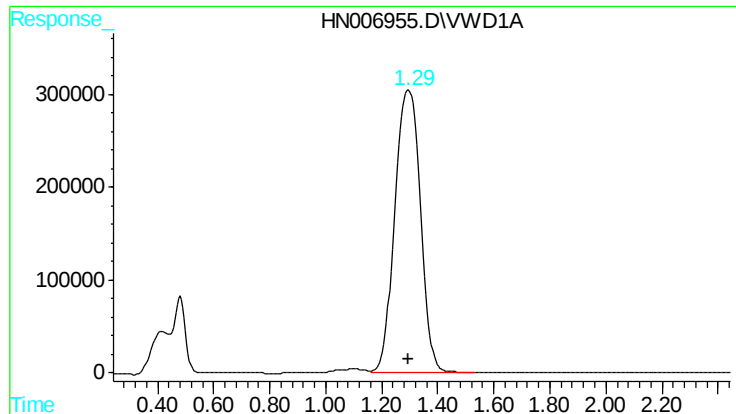

#1 4-Nitroaniline

R.T.: 1.296 min
Delta R.T.: 0.000 min
Response: 19395744
Conc: 5335.46 ug/L

Instrument :
HPLC_N
ClientSampleId :
YS19-SB19-1014